



Cite this: *RSC Appl. Interfaces*, 2026, **3**, 1298

Antibacterial surface engineering: bioinspiration from leaves to medical devices

Dannielle M. Cox-Pridmore,^{abc} Eleanor Mishra,^{cde}
Mark Webber^{bc} and Sheng Qi^{id} *^{acf}

Healthcare-acquired infections (HAIs) and the rise of antimicrobial resistance (AMR) are critical global health challenges, necessitating innovative solutions to combat pathogenic bacteria. Traditional approaches, such as antibiotics and chemical disinfectants, are increasingly ineffective due to the rapid evolution of resistant strains and their associated side effects and environmental impacts. The development of antimicrobial physical surface design strategies presents a promising alternative for reducing microbial colonisation and transmission. This review provides a comprehensive examination of antimicrobial surface geometries and topographies, focusing on physical surface strategies that prevent bacterial adhesion and biofilm formation. Inspired by naturally occurring structures such as insect wings and lotus leaves, these engineered surfaces employ nano- and micro-scale patterning to exert mechanical forces that disrupt microbial cells through membrane rupture or inhibit their attachment by limiting surface area for successful adhesion. We discuss key fabrication methods, mechanisms of action, material considerations, and clinical relevance, while also addressing challenges such as scalability, durability, and regulatory issues. By highlighting both the potential and limitations of physical surface modifications in healthcare environments, this review aims to inform future research and promote the integration of surface-based strategies in the design of next-generation medical devices and high-touch clinical surfaces.

Received 26th January 2026,
Accepted 13th April 2026

DOI: 10.1039/d6lf00022c

rsc.li/RSCApplInter

1. Introduction

1.1. Bacterial biofilms and infection

Bacteria are a family of single-cell microorganisms that play a crucial role in a wide array of biological processes, environmental cycles, and technological applications. Their remarkable ability to adapt to various environments, coupled with their metabolic diversity, makes them essential for maintaining ecological balance and supporting life on Earth. However, some bacteria are pathogenic, resulting in harmful infections, and therefore, are a major focus of medical research and public health efforts.^{1–3}

It is well established that bacteria can efficiently colonise surfaces and form a biofilm rather than dwelling in a planktonic state,^{4,5} with current estimates suggesting that up to 80% of bacteria reside in biofilms.⁶ A biofilm (Fig. 1) is a complex, structured community of bacteria encased in a self-produced matrix of extracellular polymeric substances (EPS), composed of polysaccharides, proteins, and nucleic acids,⁷ that adhere to living or inert surfaces such as medical devices, for example, catheters, implants, and prosthetics.^{8–10}

Biofilm formation is a dynamic, multistage process that begins with the reversible attachment of planktonic (free-floating) microorganisms to the surface. This transitions to irreversible attachment, and bacteria begin to secrete EPS, forming a matrix that encases the cells and anchors them to the surface. As the biofilm grows and matures, microbial cells communicate with each other through quorum sensing to coordinate their activities, such as nutrient acquisition, metabolism, and defence mechanisms.¹¹ The protective EPS barrier, reduced growth rates, high density of the bacterial cells, and the prevalence of persister cells within the biofilm enhance resistance to antibiotics, disinfectants, host immune defences, desiccation, and nutrient limitations, compared to planktonic bacteria. Eventually, environmental cues trigger the dispersion of cells from the biofilm, allowing them to colonise new surfaces and repeat the cycle. This entire

^a School of Chemistry, Pharmacy and Pharmacology, Faculty of Science, University of East Anglia, Norwich Research Park, Norwich, NR4 7TJ, UK

^b Quadram Institute, Rosalind Franklin Road, Norwich Research Park, NR4 7UQ, UK

^c Centre for Microbial Interactions, Norwich Research Park, Norwich NR4 7UG, UK

^d Department of Respiratory Medicine, Norfolk & Norwich University Hospital, Norwich, NR4 7UY, UK

^e Faculty of Medicine & Health Sciences, University of East Anglia, Norwich Research Park, Norwich, NR4 7TJ, UK

^f School of Pharmacy and Pharmaceutical Sciences, Institute of Systems, Molecular and Integrative Biology, University of Liverpool, Liverpool, L69 3GE, UK.

E-mail: sheng.qi@liverpool.ac.uk

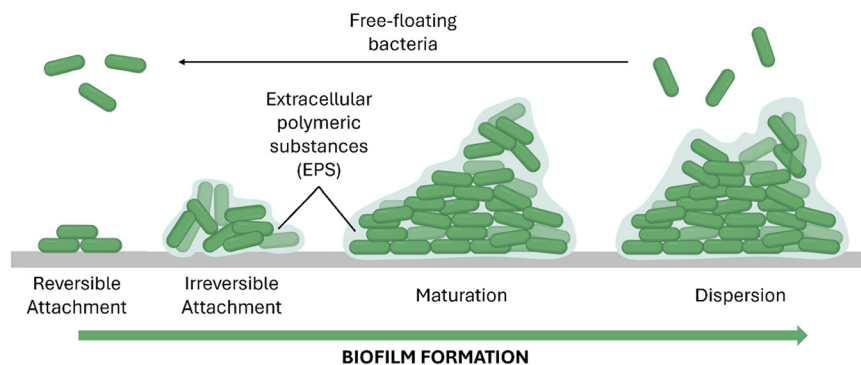


Fig. 1 A schematic of bacterial adhesion and biofilm formation on a surface. Free-floating bacteria land on the surface, produce EPS, and become part of a resilient bacterial biofilm. Eventually, bacteria will disperse, resulting in the colonisation of new environments. Created using BioRender.

process and the protective environment that the biofilm provides^{12–14} contributes to the persistence and chronicity of biofilm-associated infections,^{15–18} which are challenging to treat and eradicate.^{19–24}

In healthcare settings, opportunistic pathogens frequently contribute to healthcare-associated infections (HAIs).^{25,26} HAIs are infections that patients acquire while receiving treatment for medical or surgical conditions within a healthcare setting, such as hospitals, outpatient clinics, nursing homes, and long-term care facilities. HAIs significantly increase medical care costs, length of hospital stays, and mortality rates. It is predicted that nearly 3.5 million people could lose their lives due to HAIs every year, up to 2050.²⁷ Approximately 80% of HAIs can be attributed to biofilms, therefore, representing one of the greatest challenges in healthcare.^{7,24,28}

1.2. Chemical approaches for managing bacteria and biofilms

Antibiotics are medications that are used to treat or prevent some types of bacterial infection. The extensive use of antibiotics is due to their broad range of effects, which include blocking the formation of bacterial cell walls, damaging cell membrane integrity, interfering with the production of nucleic acids and proteins, and disrupting essential metabolic processes. Therefore, it represents a first-choice drug for patients with an infection.^{29–31} However, due to the protective nature of biofilms, these infections are often resistant to conventional antibiotics.¹⁴ Therefore, the misuse and overuse of antibiotics have encouraged the development of antibiotic-resistant bacteria, further contributing to the development of chronic, life-threatening infections.^{32,33}

Alongside antibiotics, disinfectants and chemical sanitisers are widely used to manage bacteria within healthcare settings to reduce HAI incidence. However, repeated use is practically and economically challenging. Moreover, there is growing evidence that extended interaction with such chemicals for sanitisation purposes (chlorine, hydrogen peroxide, sodium hypochlorite, ethanol) can lead to the enhanced probability of contracting long-term heart and lung diseases.^{34–37}

Another chemical-based approach worthy of attention within healthcare settings is the application of metal-based surface coatings.^{38,39} These coatings incorporate metal ions (e.g., silver, copper, zinc), metal oxides, or metal–organic frameworks,^{40–42} offering broad-spectrum antimicrobial activity through mechanisms such as reactive oxygen species (ROS) generation and bacterial membrane disruption.^{26,43–46} Despite their demonstrated antibacterial potential, several challenges hinder their widespread application. Ensuring stability under real-world conditions remains difficult, and the protective EPS matrix of biofilms can restrict ROS penetration. For example, silver-coated catheters are currently on the market with the ability to prevent infection for several days, but ultimately, result in biofilm formation, restricting long-term use.^{47,48} Moreover, coating efficacy is highly dependent on factors such as application method, environmental conditions, and surface cleanliness.⁴⁹ The non-selective toxicity of metals and potential for metal ion leaching can lead to cytotoxicity and adverse host effects, posing significant barriers to clinical translation.^{50,51}

Due to the nature of antibiotics, disinfectants, and metal-based coatings putting selective pressure on microbes, they result in increased risk of antimicrobial resistance (AMR) development.^{39,52–55} AMR poses a severe and escalating global health threat, pushing 24 million more people into extreme poverty in the next decade, and by 2050, will result in 10 million deaths annually and have an economic impact of \$100 trillion.^{56–58} The spread of AMR endangers essential medical procedures, such as surgeries and chemotherapy, which rely on effective infection control; therefore, the development of new biofilm-prevention methods and rigorous stewardship of existing antimicrobials are crucial.

Given this tremendous concern, there is an increasing motivation for designing and developing antimicrobial surfaces that provide a sustainable approach to prevent biofilm formation and the spread of infections, while reducing our reliance on antibiotics and harsh chemical agents. Several reviews explore chemical-based approaches in more depth.^{59–62} This review focuses primarily on physical approaches to managing bacteria and biofilms.

2. Physical approaches for managing bacteria and biofilms

2.1. Background

Using surface topography is an innovative approach to achieving antibacterial effects without relying on chemical agents. By designing surfaces with specific patterns, such as ridges, spikes, or pillars, bacteria are prevented from adhering, colonising, and forming a stable connection to the surface to form a biofilm. Antibacterial surfaces can be broadly classified as either antibiofouling, which repels or resists bacterial attachment, or bactericidal, which actively kills bacteria. In some instances, an antibacterial surface may exhibit both antibiofouling and bactericidal characteristics.^{59,63–68} This strategy offers an alternative approach to traditional chemical-based methods to manage bacterial load. Such engineered topographies can be applied to medical devices, implants, and high-contact surfaces to maintain sterility and minimise infection risks within healthcare settings.

2.2. Nature-inspired biomimetic antibacterial physical strategies

Nature is an unexhausted source of inspiration for scientists and engineers, particularly for the development of biomimetic antibacterial and antifouling designs. Some natural surfaces have developed the ability to resist or prevent bacterial colonisation and biofilm formation.⁶⁹ These surfaces include certain plant leaves, gecko feet, shark skin, insect wings, fish scales, and spider silk, which are frequently

studied for their self-cleaning, low-adhesive, and superhydrophobic properties, many of which also confer antibacterial capabilities.^{70,71}

Several natural surfaces prevent microbial attachment through purely physical means, as shown in Table 1. For instance, cicada wings feature high-aspect-ratio nanopillar arrays that mechanically rupture bacterial membranes upon contact. As shown in Fig. 2, *P. aeruginosa* loses shape and turgor due to penetration from the wing features.⁷² Unlike chemical coatings, these surfaces rely on mechanical interactions to exert their bactericidal effects. Similarly, shark skin is composed of dermal denticles, which create a rough surface topography that reduces hydrodynamic drag and, therefore, microbial adhesion. The structured patterns alter local fluid dynamics and create a level of turbulence, potentially minimising the time microorganisms remain in contact with the surface and facilitating their removal.^{73,74} These principles have been commercially translated, most notably being Sharklet®, which replicates key features of shark skin topography to reduce bacterial attachment. Sharklet® is a synthetic surface fabricated *via* photolithography that mimics the ordered microtopography of dermal denticles using interlocking diamond-shaped riblets. The efficacy of Sharklet® surface patterns has been reviewed in more depth and demonstrates the varying efficacy depending on the microbial species (47–99% reductions),^{63,75–78} underscoring the inherent complexity of biological systems and the different ways different bacterial species will respond to the same surface.

It is important to note that the experimental methods to understand bacterial behaviour vary, reflecting a lack of

Table 1 Examples of naturally occurring antibacterial physical surfaces

Surface	Features	Fabrication technique	Antibacterial activity	Ref.
Lotus leaf (<i>Nelumbo nucifera</i>)	Micro-papillae, 100 µm height and 100 µm spacing. Wax crystalloids, 1–5 µm in height. Tabular and convex papillae, 30–50 µm length and 10–30 µm width. Superhydrophobic (WCA = 162°)	Natural	Antibiofouling	118–120
Taro leaf (<i>Colocasia esculenta</i>)	Nano (<0.5 µm), micro (>0.5–10 µm) and macro topographies (>10 µm). Superhydrophobic (WCA = 164°)	Natural	Antibiofouling	118, 121, 122
Shark skin (<i>Carcharodon carcharias</i>)	Dermal denticles, 26.8 µm height, 99.5 µm spacing	Natural	Antibiofouling	123
Shark skin (<i>Centrophorus granulosus</i>)	Dermal denticles, 15.8 µm height, 136.8 µm spacing	Natural	Antibiofouling	123
Cicadas	<i>Megapomponia intermedia</i> , pillars, 241 nm height, 156 nm diameter, 165 nm spacing <i>Ayuthia spectabile</i> , pillars, 182 nm height, 207 nm diameter, 251 nm spacing <i>Cryptotympana aguila</i> , pillars, 182 nm height, 159 nm diameter, 187 nm spacing	Natural	Bactericidal against Gram-negative bacteria (<i>Pseudomonas fluorescens</i>)	124
Cicada wing (<i>Psaltoda claripennis</i>)	Nanoneedles, 200 nm height, 170 nm spacing. Superhydrophobic (WCA = 158–159°)	Natural	Bactericidal against Gram-negative bacteria (<i>Pseudomonas aeruginosa</i>)	67, 125
Gecko skin (<i>Lucasium</i> sp.)	Spinule structures, 3000 nm height, 500 nm spacing, tip radius of curvature <20 nm. Superhydrophobic (WCA = 150–155°)	Natural	Bactericidal against Gram-negative bacteria (<i>Porphyromonas gingivalis</i>)	114
Dragonfly wing (<i>Diplacodes bipunctata</i>)	Nanopillars, 240 nm height, 200 nm spacing. Superhydrophobic (WCA = 153°)	Natural	Bactericidal against Gram-positive (<i>Bacillus subtilis</i>) and Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	126–128

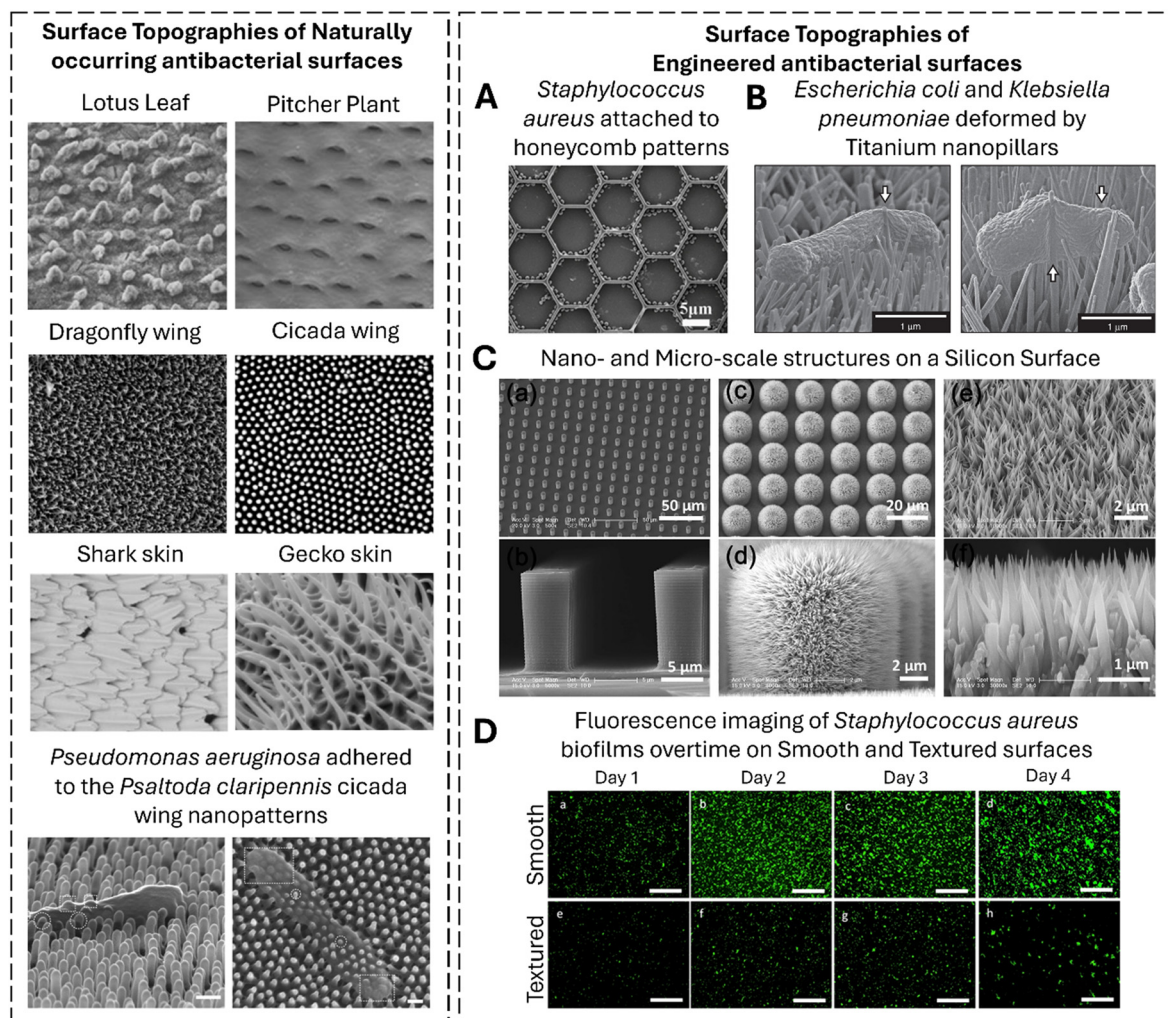


Fig. 2 Naturally occurring and engineered surface topographies that demonstrate antibacterial behaviour. (Left) SEM images of naturally occurring surface features found on the lotus leaf,¹¹⁰ pitcher plant,¹¹¹ dragonfly wing,¹¹² cicada wing,¹¹³ shark skin,⁷³ and gecko skin,¹¹⁴ including *P. aeruginosa* losing shape and turgor on cicada wing patterns, with outlines highlighting penetration and perturbation. Scale bars = 200 nm.⁷² (Right) SEM images of engineered surface features to demonstrate antibacterial behaviour. (A) 5 μm honeycomb-like patterns result in the random distribution and adhesion of *S. aureus* to the side walls.¹¹⁵ (B) *S. aureus* and *P. aeruginosa* (false coloured red) attached and ruptured by gold nanopikes.¹¹⁶ (C) Micro- and Nano-scale structures patterned on a silicon surface.¹¹⁰ (a) and (b) are microscale structures patterned surfaces; (c) and (d) are dual-scale structures patterned surface; (e) and (f) are pure nanoscale structure patterned surface ((a), (c) and (e) are images tilted at an angle of 45°, and (b), (d) and (f) are images at cross-sectional views). (D) Fluorescence images showing the reduction of *S. aureus* biofilms on textured surfaces (e–h) compared with smooth surfaces (a–d) after 1, 2, 3, and 7 days. Scale bar = 100 μm .¹¹⁷ Images were reprinted (adapted) with permission.¹¹⁰ Jiang et al., (2020). Copyright 2020, Elsevier.¹¹¹ Moran et al., (2010), licensed under CC.¹¹² Kamarajan et al., (2020), licensed under CC.¹¹³ Pogodin et al., (2013). Copyright 2013, Biophysical Society.⁷³ Chien et al., (2020). Copyright 2020, Elsevier.¹¹⁴ Watson et al., (2015). Copyright 2015, Elsevier.⁷² Velic et al., (2021). Copyright 2021, Elsevier.¹¹⁵ Yang et al., (2015). Copyright 2015, Elsevier.¹¹⁶ Elbourne et al., (2019), licensed under CC.¹¹⁷ Khursheed et al., (2024), licensed under CC.

standardisation and methodological uniformity across studies,⁷⁹ as shown in Tables 2 and 3. Commonly used methods to assess the antibacterial activity of surfaces include viability staining with fluorescent dyes such as SYTO 9 and propidium iodide (PI), colony-forming unit (CFU) counts, and imaging techniques such as confocal laser scanning microscopy (CLSM), fluorescence microscopy, and scanning electron microscopy (SEM). These approaches can provide complementary information, but each technique has notable limitations. CFU counts enable quantification of viable, culturable bacteria; however, this method often

underestimates bacterial survival due to the presence of viable but non-culturable (VBNC) populations or incomplete detachment of biofilms from surfaces.^{80–83}

Fluorescence-based assays and microscopy allow visualisation of cell viability and spatial distribution. CLSM in particular can provide three-dimensional information on biofilm structure, whereas SEM offers high-resolution imaging of bacterial morphology and surface interactions.^{84–86} Fluorescent staining approaches can be influenced by staining conditions such as dye concentration, incubation time, and biofilm thickness,

Table 2 Examples of bactericidal physical surface topographies. *Material chemistry may synergise with surface structures to demonstrate antibacterial effect. Propidium iodide (PI). Colony forming unit (CFU). Confocal laser scanning microscopy (CLSM). Scanning electron microscopy (SEM). Atomic force microscopy (AFM)

Surface	Features	Fabrication technique	Antibacterial activity testing methods	Bactericidal efficacy	Ref.
Black silicon	Nanograss, 500 nm height, 20–80 nm diameter. Hydrophilic (WCA = 80°)	Reactive ion etching	SYTO 9/PI CLSM CFU counts	Effective against Gram-positive (<i>Bacillus subtilis</i>) and Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	126
Black silicon	Nanograss, 4 µm height, 220 nm diameter Superhydrophobic (WCA = 154°)	Deep reactive ion etching	SYTO 9/PI Fluorescence microscopy CFU counts	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	140
Black silicon	Nanopillars 280 nm height, superhydrophilic (WCA = 8.4° ± 2.1°) 430 nm height, hydrophilic (WCA = 12.4° ± 1.2°) 610 nm height, superhydrophilic (WCA = 9.9° ± 1.0°)	Plasma etching	SYTO 9/PI CLSM SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	141
Diamond-coated* black silicon	Nanoneedles, 0.5–1 µm height (short needle) and 15–20 µm height (long needle)	Plasma etching and vapour deposition	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	142
Cicada-inspired diamond* surface	Nanocones with sharp tips, 3–5 µm height, 10–40 nm tip diameter, 350 nm–1.2 µm nanocone width	Microwave plasma chemical vapour deposition and reactive ion etching	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	143
Dragonfly-inspired titanium (Ti)* nanopatterned array	Nanowires, average diameter 40.3 nm. Hydrophilic (WCA = 73°)	Hydrothermal etching	SYTO 9/PI CLSM SEM	Effective against Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	144
Cicada wing-inspired Ti* columns	Nanocolumns, 478 ± 6 nm height. Nano-sized grains, 33 ± 7 nm width. 26 ± 3 nm (R_q) surface roughness Hydrophilic (WCA = 41.48° ± 0.83°)	Glancing angle sputter deposition	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-negative (<i>Escherichia coli</i>) bacteria	145
Ti alloy* surface	Nanospikes, 2 µm height, 10 nm diameter, 2 µm spacing	Anodisation	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) bacteria	146
Ti alloy* surface	Nanospikes, 20 nm diameter	Thermal oxidation	SYTO 9/PI Fluorescence microscopy PrestoBlue®	Effective against Gram-negative (<i>Escherichia coli</i>) bacteria	147
Cicada-inspired Titania* nanowire arrays	Nanowires Brush type: 100 nm diameter Niche type: 10–15 µm diameter	Hydrothermal process	SYTO 9/PI Fluorescence microscopy PrestoBlue® SEM	Effective against motile bacteria (<i>Pseudomonas aeruginosa</i> , <i>Escherichia coli</i> and <i>Bacillus subtilis</i>)	148
Titania* micro-nanopillar arrays	Pillar array sizing 20 µm, 10 µm, 5 µm, 2 µm, 1.4 µm, 1.2 µm, 1.0 µm, 0.8 µm, and 0.6 µm Hydrophilic (WCA < 90°)	Photolithography, RF magnetron sputtering and thermal oxidation	SYTO 9/PI CLSM SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	149

Table 2 (continued)

Surface	Features	Fabrication technique	Antibacterial activity testing methods	Bactericidal efficacy	Ref.
Aluminium (Al 6063 alloy) nanostructured surface	Etching time: 0.5 h, 69.9 ± 5.3 nm (R_{rms}), hydrophilic (WCA = $28.2^\circ \pm 3.3^\circ$) 1 h, 133.6 ± 36.1 nm (R_{rms}), hydrophilic (WCA = $21.8^\circ \pm 4.7^\circ$) 3 h, 995 ± 114.7 nm (R_{rms}), hydrophilic (WCA = $17.7^\circ \pm 4.3^\circ$)	Wet chemical etching	SYTO 9/PI Fluorescence microscopy	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	150
Cicada wing-inspired PMMA nanopatterned surface	Nanopillars, 200–300 nm height, 70–215 nm diameter, 130–380 nm spacing	Nanoimprint lithography	SYTO 9/PI Fluorescence microscopy CFU counts SEM AFM	Effective against Gram-negative (<i>Escherichia coli</i>) bacteria	151
Poly-L-lactic acid (PLLA) surface	Cylindrical micropillars, 40 μm height, 40 μm width decorated with nanostructures. Hydrophobic (WCA $>100^\circ$)	Nanoimprint lithography	ISO 207043:2007 CFU counts SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	152
Polycarbonate surface	Nanopillars arrays, 143–408 nm height, 100–313.9 nm spacing Hydrophobic	Nanoporous anodic aluminium oxide (AAO) template-assisted hot embossing and wet etching	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-negative (<i>Escherichia coli</i>) bacteria	153
Gecko skin-inspired nano-spinules	Spinules, 1–4 μm height, 600 nm spacing. Hydrophobic (WCA = 134°)	Nano-templating	SYTO 9/TO-PRO-3 Laser confocal microscopy SEM	Effective against Gram-positive bacteria (<i>Lactobacillus</i>)	154
Cicada wing-inspired gold (Au)* nanopatterns	Nanopillars (100 nm height, 50 nm diameter) Nanorings (100 nm height, 100–200 nm diameter) Nanonuggets (100 nm height, 100–200 nm diameter)	Electrodeposition and plasma etching	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) bacteria	155
PDMS or PMMA nanopatterns	Moth-eye nanocones, 250 nm diameter at the base and 80 nm on the top, 350 nm height and 250 nm spacing	PDMS-soft lithography PMMA-thermal nanoimprint lithography	SYTO 9/PI Fluorescence microscopy SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	156

which may affect dye penetration and lead to misinterpretation of viability.^{87–90} Microscopy-based techniques rely on image processing or fluorescence intensity measurements that can vary depending on imaging parameters. In addition, SEM requires extensive sample preparation, which may alter biofilm structure.⁹¹ A further challenge across these methods is the lack of standardised protocols for dye concentrations, incubation conditions, and quantification approaches, making comparisons between studies difficult. Consequently, while these techniques are widely used to evaluate antibacterial surfaces, careful methodological control and the combination of multiple complementary assays are often necessary to obtain reliable and reproducible assessments of antibacterial performance.

Biomimetic replication of features seen in nature has led to promising engineered surfaces. For example, Kumar and Bhardwaj (2020) replicated the hierarchical structure of the taro leaf using photolithography, achieving static contact angles up to 148° by mimicking the dual-scale hexagonal and flake-like microstructures.⁹² However, traditional fabrication methods, such as photolithography, make the whole process costly and time-consuming, with limited scalability. Therefore, there has been a lack of commercialisation of such surfaces. However, the research and these examples underscore the effectiveness of biologically inspired surface topographies in resisting bacterial colonisation and biofilm development.

For antibacterial surface topographies to achieve translational and commercial impact, scalable and high-throughput

Table 3 Examples of antifouling physical surface topographies. *Material chemistry may synergise with surface structures to demonstrate antibacterial effect. Propidium iodide (PI). Confocal laser scanning microscopy (CLSM). Scanning electron microscopy (SEM). Colony forming unit (CFU). Green fluorescent protein (GFP)

Surface	Features	Fabrication technique	Antibacterial activity testing methods	Antifouling efficacy	Ref.
Silicon micropillar arrays	Various sizings: 20 μm , 10 μm , 5 μm , 2 μm , 1.4 μm , 1.2 μm , 1.0 μm , 0.8 μm , and 0.6 μm Hydrophilic (WCA < 90°)	Photolithography and dry etching	SYTO 9/PI CLSM SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	180
Silicon honeycomb pattern with micro-size pores	Pore sizes: 0.5 μm , hydrophilic (WCA = 70° $\pm$ 4°) 1 μm , hydrophobic (WCA = 100° $\pm$ 2°) 3 μm , hydrophobic (WCA = 118° $\pm$ 1°) 5 μm , hydrophilic (WCA = 84° $\pm$ 2°) 10 μm , hydrophilic (WCA = 80° $\pm$ 2°)	Photolithography and deep reactive ion etching	SYTO 9 CLSM SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	115
Lotus leaf-inspired Ti* surface	Micro-grains (10–20 μm), Nano-undulations (<200 nm). Superhydrophobic (WCA = 166°)	Femtosecond laser irradiation	SYTO 17/Concanavalin A Alex Fluor 488 CLSM SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	181
Ti* mesopores	Pores, 20–25 nm diameter, $\sim$ 17 nm (R_{rms}) surface roughness	Chemical oxidation	SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	182
Lotus leaf-inspired Ti alloy* surface	Various surface textures (390 nm, 660 nm, and 1.1 μm)	Laser texturing	SEM	Effective against gram negative (<i>Escherichia coli</i>) bacteria	122
Nanostructured PMMA film	Nanopores, 460 nm depth, 300 nm spacing Hydrophobic (WCA = 114.5°)	Nanoimprint lithography	GFP-expression Fluorescence microscopy	Effective against Gram-negative (<i>Pseudomonas aeruginosa</i> and <i>Escherichia coli</i>) bacteria	183
Shark skin-replicated PMMA microstructure	Tail abdomen denticles, 164.5 μm height, 85.7 μm width, 118.8 denticles per mm^2 . Hydrophobic (WCA = 115.8°) Pectoral fin denticles, 166.2 μm height, 69.8 μm width, 83.3 denticles per mm^2 . Hydrophobic (WCA = 105.6°)	Polymer imprinting	Crystal violet	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	73
PDMS micropatterned surface	Square features, 6 μm height, 4 μm spacing Circular features, 3 μm diameter, 2 μm spacing. Ridges, 2 μm width and 3 μm -wide channels. Hydrophobic (WCA = 108.7°)	Soft lithography	Quantified manually SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i> and <i>Staphylococcus epidermidis</i>) bacteria	184
Polystyrene spheres	630–1550 nm monodisperse spheres	Colloidal crystal fabrication	Light microscopy SEM	Effective against Gram-negative (<i>Pseudomonas aeruginosa</i>) bacteria	157
Polypropylene (PP) films	Micropillars, 10 μm height, 10 μm diameter, 23 μm spacing Nanospikes, 2.2 μm height, 300 nm base diameter. Hydrophobic (WCA >100°)	Nanoimprint lithography and reactive ion etching	Touch transfer assay CFU count	Effective against Gram -ositive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	108
Shark skin-mimicked chitosan*/graphene oxide* membranes	Topographies from the skin of a basking shark (<i>Cetorhinus maximus</i>)	Negative Mold	ISO 22196 CFU count MTT assay SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) and Gram-negative (<i>Escherichia coli</i>) bacteria	185

Table 3 (continued)

Surface	Features	Fabrication technique	Antibacterial activity testing methods	Antifouling efficacy	Ref.
Nanostructure sutures	Lamella structure, 500 nm length, 100 nm thickness	Plasma etching	SYTO 9/PI Fluorescence microscopy CFU counts SEM	Effective against Gram-negative (<i>Escherichia coli</i>) bacteria	186
Structured polystyrene surface	Lamella structures, 0.47 μm width, 2 μm spacing	Direct laser interference patterning	CFU counts SEM	Effective against Gram-positive (<i>Staphylococcus aureus</i>) bacteria	187

manufacturing techniques need to be considered and used to produce nano- and micro-scale features reliably and reproducibly over large areas, with relevant materials, and on clinically relevant substrates. Roll-to-roll nanoimprint lithography offers significant promise, enabling continuous pattern transfer onto polymer films at industrial speeds with high reliability and relatively low cost per unit. In combination with nanocoining, the manufacturing can also overcome the high cost associated with a master mould. This approach is particularly attractive for disposable medical products, wound dressings, and device surfaces, where large-area replication and throughput are critical.^{93–95} Similarly, laser-based methods, such as laser-induced periodic surface structures (LIPSS), provide a single-step method for creating features directly onto metallic or polymeric surfaces. LIPSS is especially relevant for orthopaedic implants, surgical tools, and catheter components, as it can be applied to complex geometries and hard materials while allowing spatial control of patterning.^{96–99} Other scalable approaches, including injection moulding with textured moulds,^{100,101} hot embossing,^{102,103} and reactive ion etching,^{104,105} also present industrially viable routes, particularly when integrated into existing medical device manufacturing pipelines.

However, for these techniques to be clinically feasible, they must demonstrate not only pattern uniformity and reliability, but also compatibility with regulatory requirements, sterilisation processes, mechanical durability, and cost constraints. Moreover, reproducibility across large production batches and the ability to pattern three-dimensional, curved, or flexible substrates remain practical challenges. A deeper consideration of manufacturing scalability, including tooling lifetime, cycle time, material compatibility, and quality control metrology, will therefore be essential to bridge the gap between laboratory proof of concept research and commercially available antibacterial medical devices and healthcare equipment. Detailed reviews of fabrication strategies and manufacturing techniques are available.^{106,107}

As mentioned, for physical antibacterial topographies to achieve translational feasibility, they must demonstrate durable antimicrobial efficacy alongside mechanical and chemical stability under real-world conditions. In clinical and industrial settings, the topographies would be routinely exposed to extensive cleaning procedures, repeated sterilisation cycles, and frictional wear. Francone *et al.*, (2021) fabricated patterned

polypropylene and conducted washability tests mimicking hospital-specific cleaning protocols, which demonstrated that the features of the surface, such as topography, water contact angle, and gloss, remained unchanged despite intensive physical and chemical cleaning procedures over time.¹⁰⁸ This demonstrates promise for the application of nano- and micro-patterning within clinical settings. Theoretically, if the patterns are not damaged, the surface can be reused indefinitely when cleaned.¹⁰⁹ However, from this literature review, it is seen that many studies show high initial promise but rarely test the durability of the features against wear, fouling, and bacterial resistance, with more research needing to be conducted within this area. Therefore, the rational design of antibacterial surface topographies must integrate considerations of mechanical durability, chemical resistance, and wear stability alongside antimicrobial performance to ensure function throughout the intended lifespan of the surface.

2.3. Bactericidal physical surface topographies

Bactericidal surface topographies are designed to actively kill bacteria through mechanical forces. These surfaces often feature nanoscale structures such as spikes, pillars, or sharp ridges that can promote adhesion and then stretch, puncture, or rupture bacterial cell membranes upon contact, as they grow, or during movement, and if the applied force exceeds their elasticity, leading to bacterial lysis and death. This deformation-stretching-torn apart effect has been observed in various engineered surfaces, including biomimetic designs inspired by cicada and damselfly wings.^{113,129,130} The ability of a bacterium to rupture due to a nanopatterned surface may also depend on the maturation stage of the cell, as shown by Truong *et al.*, (2017). The nanopillars present on the wings of the damselfly (*Calopteryx haemorrhoidalis*) exhibited the highest bactericidal activity in the early (1 hour) and late (24 hour) stationary phase of *Staphylococcus aureus* and *Pseudomonas aeruginosa*, resulting in 89.7 and 61.3% as 97.9 and 97.1% dead cells upon surface contact, respectively.¹³¹ These findings highlight that strong bacterial adherence to the nanopatterned surface is critical for effective mechano-bactericidal activity. High-aspect-ratio structures are particularly important for promoting initial

bacterial attachment, which facilitates subsequent membrane rupture, for example, hierarchical structures like two-tiered micropillar arrays.¹²⁹ The bactericidal performance of such surfaces is strongly influenced by structural characteristics, including pillar height, diameter, density, and spatial arrangement. Denser and smaller nanopillar arrays have been found to be more effective against both Gram-negative and Gram-positive bacteria compared to larger, widely spaced configurations,¹³² because they need to promote adhesion to be able to demonstrate their killing effect.

Other characteristics of bacteria, such as their motility, morphology, and size, can influence their interactions with nanopatterned surfaces. Highly motile bacteria experience greater membrane deformation due to movement across the surface, leading to increased cell rupture.¹³³ Morphological differences, such as being coccoid or rod-shaped, can impact their interactions with the same surface. The relative dimensions of bacterial cells and surface patterns are also critical. Bactericidal efficiency is enhanced when cell size exceeds the spacing between nanopatterns, allowing for direct penetration and rupture. Conversely, smaller bacterial cells may stretch or compress against the sidewalls of nanostructures, resulting in different mechanical stress responses. Kelleher *et al.*, (2016) demonstrated that surfaces with tighter nanopillar spacing and smaller feature sizes showed superior bactericidal activity compared to those with lower density and larger features.¹²⁴ Modaresifar *et al.*, (2019) systematically reviewed bactericidal nanopatterning and reported that most design parameters tend to fall within specific ranges: feature height between 100–1000 nm, diameter between 10–300 nm, and spacing less than 500 nm.¹³⁴ A variety of materials and surfaces have been explored to demonstrate bactericidal activity, for example, black silicon is widely used, which is regular silicon etched to produce nanoscale markings that make it appear black due to trapping of light.¹³⁵ In order to show the breadth of research in this area, Table 2 is generated to summarise the materials used, feature dimensions, fabrication techniques, bactericidal activity, and how it is evaluated. It explores several examples of bactericidal surface patterns with their respective features and what they are effective against.

A challenge in the field of antibacterial surface topographies is the lack of standardisation and methodological uniformity across existing studies, which significantly limits comparison, meta-analysis, and reproducibility. A critical evaluation by Redfern *et al.*, (2024) revealed substantial variation in growth conditions, controls, and analytical measurements of biofilms performed by different research groups.⁷⁹ Standardisation of microbiological practice is inherently difficult due to differences in equipment, technical expertise, and laboratory resources across institutions. Furthermore, biofilm science itself remains an evolving field, with ongoing debate regarding the most appropriate methods to grow, control, quantify, and analyse bacteria and biofilms.

In addition, there is often an inadequate characterisation of the topography. For example, relying on parameters like average roughness, which does not describe the dimensions of the pattern itself.¹³⁶ Surfaces with identical roughness values may have

different heights, widths, spacing, and shapes, which also significantly impact how bacteria interact with the surface. Researchers must provide sufficient details of topographical descriptors such as feature height, width, spacing, shape, surface chemistry, *etc.*, as well as experimental conditions such as bacterial strain selection, growth phase, inoculum density, media composition, incubation duration, and environmental parameters, in addition to reasoning behind quantitative outcome measures.

Interactions at the bacteria–surface interface are complex, dynamic, and heavily dependent on specific environmental conditions. There is no ‘one-size-fits-all’ solution with patterned surfaces, and the features need to be tailored depending on the bacterial species and the environment it will be experiencing. The optimisation of pattern design, including parameters such as feature density, stiffness, and geometry, is therefore needed to enhance the antibacterial surface performance for different bacterial species.^{137–139}

Optimal topographical design is likely to be context specific. A micro- or nano-scale pattern that reduces bacterial colonisation on a dry, high-touch hospital surface may not perform equivalently on an implanted medical device, where continuous fluid flow, immune interactions, and long-term mechanical stresses alter bacterial behaviour. Therefore, proposed best practices should not only encourage comprehensive reporting of surface parameters, microbiological conditions, and quantitative antibacterial measurements, but also require clear justification of experimental models in relation to the intended end-use environment. Establishing such a structured reporting framework would enhance reproducibility, enable meaningful comparisons, and provide a more rigorous foundation for translating antibacterial topographic surfaces into clinically and industrially relevant applications.

2.4. Antibiofouling physical surface topographies

Antifouling surface topographies are engineered to prevent bacterial adhesion and colonisation rather than directly killing the cells. The surface features often create an energetically unfavourable environment for microbial attachment, or geometries that physically limit the ability of bacteria to establish stable contact. Table 3 explores some examples of antibiofouling surfaces along with the species they are reported to be successful against. As shown, these features range from the nano- to the micro-scale; however, the broader literature provides a fragmented, often incomplete, and potentially contradictory view of antifouling features and what works best. For example, Kargar *et al.*, (2014) reported that larger spherical features delayed biofilm formation compared to smaller ones.¹⁵⁷ Yet literature often recommends smaller topographic sizes to inhibit biofilm formation.^{158,159}

Mok *et al.*, (2019) showed that concave periodic boundary geometries limited *Escherichia coli* accumulation,¹⁶⁰ while Gu *et al.*, (2017) demonstrated that hexagonally arranged topographies with optimised spacing disrupt intercellular interactions and limit biofilm formation.¹⁶¹ In another study,

Gu *et al.*, (2016) further demonstrated that bacterial orientation tends to align perpendicularly to linear patterns, with more random attachment occurring as line widths increase and approach planar surfaces.¹⁶² Ge *et al.*, (2019) attributed antibacterial efficacy (e.g., 62% reduction in *S. aureus* adhesion, and 73% reduction in *E. coli* adhesion) to the synergistic effects of reduced contact area and spatial confinement offered by pillar-based topographies.¹⁴⁹ However, it is important to note that this group used Titanium oxide, which is inherently antibacterial; therefore, potential effects may not solely be due to physical approaches. In Tables 2 and 3, an annotation (*) has been made where groups have used materials that may have particular chemistries that may synergise with surface structures to demonstrate an antibacterial effect; the result is not entirely through physical means. It is important to note that a major benefit of antibacterial activity through physical mechanisms induced by nano- and micro-scale topographies is that they do not exert selective pressure for resistance development like conventional antibiotics and other chemical-based methods do.^{163,164} However, long-term efficacy and other potential impacts require further study.^{164,165}

Antifouling topographies reduce the likelihood of biofilm formation by making it difficult for bacteria to remain anchored long enough to multiply and produce EPS, through the alteration of surface properties such as roughness, contact forces, wettability, shear stress, and fluid flow. Increased surface roughness reduces bacterial adhesion by limiting available adhesion points. The reduction in contact area also impacts surface charge accumulation and distribution, therefore, altering the attractive and repulsive forces between the bacteria and the surface.^{138,166,167} Effectively, repelling the bacteria and reducing bacterial attachment.

Wettability also plays a crucial role in antibiofouling.¹⁶⁸ Superhydrophobic surfaces (water contact angle $>150^\circ$) trap air pockets, creating a barrier against bacterial attachment, while superhydrophilic surfaces (water contact angle $<5^\circ$) form a continuous water layer that prevents direct contact with bacteria.¹⁶⁹ Hierarchical structures, such as those found on lotus leaves, exhibit extreme wettability due to the combination of micro-scale bumps and nanoscale hairs. These structures allow water droplets to bead up and roll off easily, effectively preventing bacterial colonisation through self-cleaning mechanisms. A study developing titanium-based lotus leaf-like surfaces found that bacteria were unable to adhere due to trapped air nano- and micro-bubbles, which minimised contact and imparted antifouling properties.¹⁷⁰ Ellinas *et al.*, (2017) reported that a superhydrophobic polymethyl methacrylate (PMMA) surface with a water contact angle (WCA) above 155° exhibited prolonged bacterial repellence against *Synechococcus* sp. for up to 72 hours and minimised adhesion for four days.¹⁷¹ However, superhydrophobicity typically diminishes during prolonged immersion in liquid due to air layer depletion. Therefore, careful control of feature size and surface design is essential to sustain the air layer and preserve

antibacterial efficacy, and the design must be tailored to the specific environment in which it will be applied to achieve the greatest effect.

While a substantial body of literature explores surface topographies influencing bacterial attachment and biofilm formation, considerably fewer studies focus on elucidating the underlying mechanisms responsible for these effects. A deeper mechanistic understanding of how and why specific surface features inhibit biofilm development is therefore required. One mechanism of action might be the interruption of cellular signalling. As previously mentioned, quorum sensing is a form of bacterial cell-to-cell communication.^{11,172} Disrupting signalling capabilities may, in turn, disrupt stable, long-term contact of bacteria with a surface. Recent work with *P. aeruginosa* has explored the influence of nanotopographies on quorum-sensing molecule (QSM) production and their ability to reduce major virulence pathways.¹⁷³ In addition, Romero *et al.*, (2025) were able to explore that microtopographies resulted in quorum-sensing-mediated autolubrication that inhibits early-stage *P. aeruginosa* biofilm formation. It appears that the spatial restrictions of the topographies result in the production of lubricating rhamnolipids that prevent irreversible bacterial adhesion to the surface.¹⁷⁴

Other potential methods for topographies to induce antibacterial effects include altering surface contact area, therefore reducing stable attachment and disrupting the spatial organisation required for biofilm formation. It is also seen that topographies can influence hydrodynamic forces in the near-surface environment, increasing velocity, which can disrupt initial bacterial settlement. It is possible that the presence of patterns on the surface and their effect on the surrounding environment would influence quorum sensing by limiting the effective diffusion and local accumulation of autoinducers, preventing them from reaching the threshold concentrations necessary to trigger coordinated gene expression required for stable attachment and biofilm formation.^{175–178} Such mechanistic insights will enable a more comprehensive interpretation of existing results, provide further validation of observed antimicrobial performance, and support the rational design and broader application of topographically engineered surfaces across diverse environments.

By optimising surface topography, including feature dimensions, spacing, and wettability characteristics, antibiofouling surfaces can effectively minimise bacterial adhesion and biofilm development, providing a promising strategy for antimicrobial surface design. Recently, the use of machine learning (ML)¹⁷⁴ and artificial intelligence (AI)¹⁷⁹ to determine the best antimicrobial shapes and features promises accelerated discovery. Yet these methods are limited by the complexity of biological systems, which are difficult to emulate, and the lack of standardised data on topographies and their performance, which can reduce the model's accuracy. It is essential to consider the specific type of bacteria being targeted, as well as the environmental

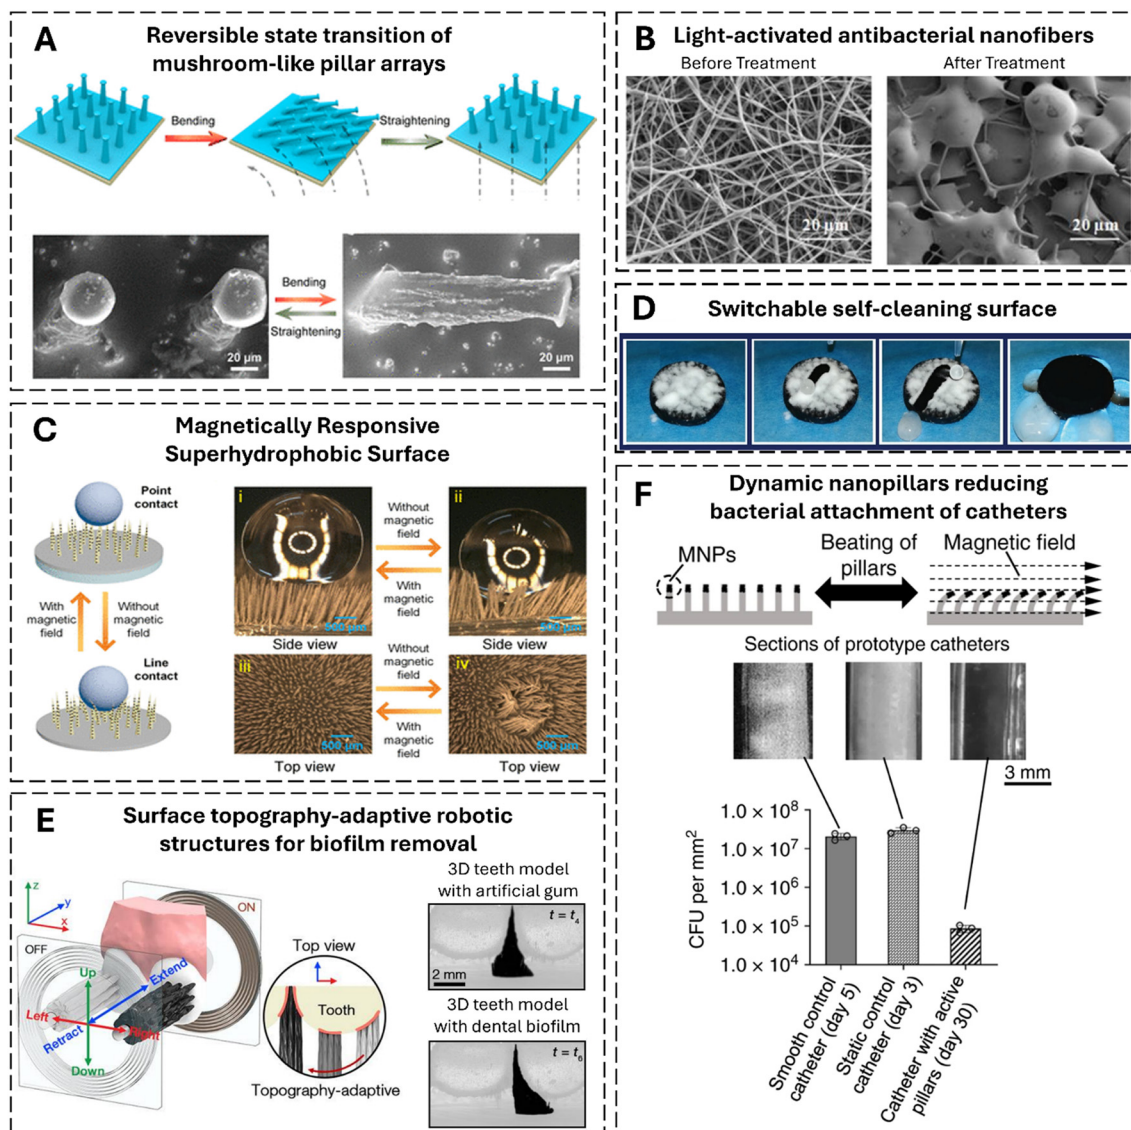


Fig. 3 Next-generation dynamic surface topography. (A) Schematic and SEM images of reversible bending and stretching of mushroom-like pillars allowing for the creation of a superamphiphobic surface.¹⁹³ (B) *meso*-Tetraphenylporphyrin (TPP)/polymethylmethacrylate (PMMA) nanofibers before and after a 20-hour light-emitting diode treatment.¹⁹⁴ (C) Schematic and optical microscopy images showing magnetorheological elastomer micropillars transformed from collapsed morphology (water-adhesive state) to the fully upright position (water-repellent state).¹⁹⁵ (D) Self-cleaning surfaces showing flour powder contamination preferentially adhering to water droplets and being successfully removed by fast drop slipping.¹⁹⁶ (E) The forward electromagnet core guides the robotic superstructure bristles across the target surface, allowing for topographical adaptation, shape variation, and deep penetration into interdental space for biofilm removal.¹⁹² (F) Schematic of magnetic nanopillars (MNPs) moving due to magnetic field. The representative images show the complete blockage (visible white substance) of static control and flat control catheters, while the prototype catheters with MNPs remained clear, resulting in lower CFU per mm².¹⁹¹ Images were reprinted (adapted) with permission.¹⁹³ Wang *et al.*, (2019). Copyright 2019, American Chemical Society.¹⁹⁴ Elashnikov *et al.*, (2016). Copyright 2016, Elsevier.¹⁹⁵ Yang *et al.*, 2018. Copyright 2018, American Chemical Society.¹⁹⁶ Děkanovský *et al.*, 2019. Copyright 2018, WILEY.¹⁹² Jun Oh *et al.*, (2024), licensed under CC.¹⁹¹ Gu *et al.*, (2020), licensed under CC.

conditions in which the surface will be applied, since these factors strongly influence the effectiveness of the design. Because they focus on prevention and reduction rather than destruction, antibiofouling topographies are especially valuable in applications where long-term resistance to biofilm growth is needed, and they can be combined with chemical coatings or bactericidal features to provide more comprehensive antibacterial protection.

3. Next-generation dynamic surface topography

Dynamic or ‘smart’ physical surface technologies represent a new frontier in antibacterial physical surface design. Unlike static topographies, these surfaces can adapt their physical properties, such as shape, size, stiffness, or wettability, in response to external stimuli like temperature, pH, light, or

mechanical force (Fig. 3). This adaptability allows them to actively resist or disrupt microbial adhesion and biofilm formation in changing environments.^{188–190} For instance, thermoresponsive coatings can switch between hydrophilic and hydrophobic states, detaching adhered bacteria upon environmental changes. Similarly, shape-memory or magnetically actuated surfaces can generate mechanical forces that physically dislodge attached cells.¹⁹¹ In addition, the development of surface topography-adaptive robotic superstructures, capable of extending and retracting to dynamically adjust their shape, length, and stiffness, offers a promising approach for effective and targeted biofilm removal.¹⁹² These dynamic systems offer a promising strategy for prolonging surface efficacy and minimising microbial resistance development by introducing unpredictable and variable adhesion conditions.

4. The advantages and limitations of physical antibacterial approaches

Using surface topography to reduce bacterial adhesion and biofilm formation within the healthcare sector offers several significant advantages. Enhanced infection control is a primary benefit, as physical antibacterial strategies can substantially lower the risk of HAIs by creating surfaces inherently resistant to bacterial colonisation. This is especially crucial on medical devices and in hospitals and clinics, where stringent infection control is essential.^{60,108,197} Surface topographies could be strategically implemented on high-risk areas to passively reduce bacterial attachment and biofilm formation, thereby lowering the risk of pathogen transmission without reliance on reapplying chemical antimicrobial agents.

Physical surface strategies often exhibit broad-spectrum activity, being effective against a wide range of bacterial species, including both Gram-positive and Gram-negative bacteria, which is advantageous in diverse healthcare environments.^{198,199} Furthermore, because these strategies do not depend on specific molecular targets, bacteria are less likely to develop resistance, thereby mitigating the growing issue of AMR.^{200–202}

Environmentally, physical approaches are more sustainable and eco-friendlier, as they do not involve the release or leaching of potentially harmful chemicals or metals over time.^{108,203,204} This makes them particularly suitable for applications where biocompatibility is crucial, such as in medical implants. With recent research supporting the use of topographies to control bacterial colonisation while supporting mammalian cell attachment and tissue integration.^{106,156}

Lastly, the versatility of physical antibacterial techniques allows their application to a wide range of materials and devices, including metals, polymers, and ceramics, allowing for tailoring and engineering to suit specific applications and environments, and the creation of customised antibacterial solutions.¹⁹⁸

Despite these advantages, there are also notable challenges in implementing these strategies. Manufacturing process considerations need to be made to ensure the pattern chosen is scalable, as techniques such as lithography, plasma treatments, or laser ablation might be intricate, time-consuming, and costly, which may limit large-scale applications.^{205,206} Integrating these technologies into existing healthcare infrastructure could be complex, necessitating substantial modifications to current practices and equipment. In turn, this can result in a high initial cost for implementation, due to the need for specialised equipment and processes, which can be a barrier to widespread adoption, particularly in resource-limited settings.

Due to the success of patterning surfaces to demonstrate antibacterial effects *in vitro*, various trials have explored their use *in vivo*. A review exploring nanopatterned titanium implants showed that effectiveness varied between preclinical studies and the *ex vivo* and *in vivo* experiments. Even though antibacterial activity was often seen in comparison to the control, it was noted that the patterns were not sufficient to target chronic bone infections.²⁰⁷ Patterning of surfaces should not be seen as a replacement for antibiotics or cleaning methods, but as an additional measure to provide bacterial colonisation and biofilm control. While physical approaches can be effective, their efficacy might be lower compared to strong chemical or antibiotic treatments, especially in environments with high bacterial loads or where other factors, such as nutrient availability, promote biofilm growth. Unlike chemical disinfectants, which kill bacteria quickly on contact, physical antibacterial surfaces often take time to work by preventing adhesion and colonisation over time, potentially limiting their effectiveness in situations requiring immediate bacterial eradication.

Moreover, *in vivo* applications, such as implanted medical devices, introduce additional challenges, such as micromotion at the tissue-implant interface, protein adsorption, and inflammatory responses that may progressively alter surface architecture. The durability of topographies in *in vivo* settings has yet to be extensively studied, but there is the risk of surface fragmentation, which could cause the loss of antibacterial activity over time and cytotoxicity to mammalian cells.^{109,208} Furthermore, surface topography may wear down due to mechanical abrasion, chemical exposure, or environmental factors, leading to reduced antibacterial effectiveness.⁵⁹ While surface roughness can deter bacterial adhesion, excessively rough surfaces might trap debris or promote biofilm accumulation in surface irregularities, counteracting the intended antimicrobial effects. Ensuring consistent effectiveness may require regular maintenance and monitoring. In addition, new physical antibacterial technologies may face regulatory hurdles that can delay their market introduction, as they must undergo rigorous testing and approval processes to meet safety and efficacy standards.

While physical antibacterial approaches show great potential, challenges remain in optimising surface design for

long-term effectiveness. Superhydrophobicity, for example, may degrade due to air layer depletion, reducing its antifouling capabilities. Potential future research could focus on developing robust, switchable surfaces that maintain their antibacterial properties under varying environmental conditions. Additionally, further studies are needed to refine the exact dimensions for maximal antibacterial efficacy while ensuring compatibility with biomedical and industrial applications and processes.

By harnessing physical antibacterial strategies, researchers can develop innovative and physical surface-modification solutions to mitigate bacterial contamination, offering promising advancements in healthcare.

5. Combination approaches

Recent research suggests that the most promising route for effective and durable bacterial control is the strategic combination of approaches,²⁰⁹ such as surface topography with chemical-based methods. While nanoscale or microscale surface structures can mechanically disrupt bacterial membranes, inhibit adhesion, and delay biofilm formation, these effects alone may be insufficient under complex biological or environmental conditions like healthcare settings. Therefore, coupled with approaches like antibiotics, chemical disinfectants, and antibacterial metals, can yield synergistic effects, enhancing both immediate bactericidal activity and long-term biofilm resistance. Physical structures can reduce bacterial load and delay colonisation, while potentially decreasing the dosage and frequency of chemical agents.^{39,210–213} This combined strategy not only improves performance¹¹⁷ but also helps lessen issues such as toxicity and the growing concern of AMR, ultimately decreasing our reliance on chemical-based interventions alone. Nonetheless, significant challenges remain, particularly concerning large-scale implementation, ensuring broad-spectrum efficacy, and preventing resistance that may emerge due to the inherently resilient nature of biofilms.^{15,214} More research is required, but this multimodal strategy represents a promising design principle for next-generation antimicrobials in healthcare settings.

6. Conclusions

Surface topography offers a promising, passive, and durable antibacterial strategy. By mimicking naturally occurring antibacterial surfaces, such as insect wings or plant leaves, engineered micro- and nano-scale structures can physically deter bacterial adhesion, proliferation, and biofilm formation. However, the effectiveness of these topographies is highly context-dependent, varying with bacterial species, surface chemistry, and environmental conditions. Different bacterial species exhibit distinct adhesion behaviours and biofilm-forming capacities depending on their shape, size, motility, and surface-sensing mechanisms. Consequently, surface designs must be tailored to specific applications,

considering the dominant bacterial species likely to colonise a given medical device or environment.

Design strategies should also consider whether the intended outcome is antifouling (preventing attachment) or bactericidal (killing adhered bacteria). For instance, antifouling surfaces may be more beneficial for permanent implants to reduce biofilm formation associated with chronic infection, while bactericidal topographies may be more suitable for high-risk zones where sterilisation opportunities are limited. Although the antibacterial performance of such biomimetic surfaces has been well documented, the underlying mechanisms of action, particularly under dynamic, real-world conditions, remain an area of active research.

The successful implementation of topographical strategies also depends on practical and engineering considerations, including scalability, fabrication precision, long-term durability, and resistance to wear. Addressing these challenges requires systematic studies to develop a comprehensive library of well-characterised surface architectures, mapping their effects across bacterial species and environmental conditions. By first establishing a reliable experimental dataset, more effective ML and AI tools can be developed.

The current limiting factor of predictive models of antibacterial surface topographies is the lack of readily available, standardised, and high-quality datasets that capture the complexity of interfaces between bacteria and the patterned surface. Current research focuses narrowly on single outcome measures such as CFU counts or simple surface descriptors like roughness average. In addition, many studies are conducted under static, idealised laboratory conditions, often over 24 hours, which do not reflect physiologically relevant environments over time, leading to limited models. It is also important to note the continually evolving and complex nature of biological systems, and therefore, these datasets need to be continually updated to improve the model's accuracy. These predictive technologies in turn could accelerate surface design and screening, with the combination of resources helping guide the rational design of application-specific surfaces for medical devices and hospital infrastructure.

In summary, while physical antibacterial approaches offer substantial benefits, such as reduced antibiotic dependence, lower resistance risk, and sustained efficacy, they also face limitations related to manufacturing complexity, cost, and maintenance. Future advances are likely to emerge from dynamic surface topographies that can adapt, or combination approaches, where physical topographies are combined with chemical agents such as metal-based coatings or antibiotics to achieve synergistic, long-lasting protection. Translating these technologies into clinical practice will require continued interdisciplinary research focused on biocompatibility, long-term stability, and scalability. Ultimately, integrating topographical engineering with complementary antimicrobial strategies represents a critical

frontier in developing safer, infection-resistant surfaces and healthcare environments.

Conflicts of interest

All authors can confirm that we have no conflicts of interest to declare.

Data availability

All data supporting the findings of this study are contained within the article. This includes both original data generated in the course of the research and previously published data cited in the references.

Acknowledgements

We would like to thank the funding support from the Medical Research Council (MRC) (MR/X502972/1) and the Impact Acceleration Account (IAA) fund of the University of East Anglia.

References

- 1 S. Baron, *Medical Microbiology*, University of Texas Medical Branch at Galveston, Galveston (TX), 1996, 4th edn, PubMed PMID: 21413252.
- 2 A. Gupta, R. Gupta and R. L. Singh, Microbes and Environment, in *Principles and Applications of Environmental Biotechnology for a Sustainable Future*, Springer Singapore, Singapore, 2017, pp. 43–84, DOI: [10.1007/978-981-10-1866-4_3](https://doi.org/10.1007/978-981-10-1866-4_3).
- 3 J. Soni, S. Sinha and R. Pandey, Understanding bacterial pathogenicity: a closer look at the journey of harmful microbes, *Front. Microbiol.*, 2024, **15**, 1370818, DOI: [10.3389/fmicb.2024.1370818](https://doi.org/10.3389/fmicb.2024.1370818), PubMed PMID: 38444801.
- 4 C. E. Zobell and E. C. Allen, The Significance of Marine Bacteria in the Fouling of Submerged Surfaces, *J. Bacteriol.*, 1935, **29**(3), 239–251, DOI: [10.1128/jb.29.3.239-251.1935](https://doi.org/10.1128/jb.29.3.239-251.1935).
- 5 C. E. Zobell, The Effect of Solid Surfaces upon Bacterial Activity, *J. Bacteriol.*, 1943, **46**(1), 39–56, DOI: [10.1128/jb.46.1.39-56.1943](https://doi.org/10.1128/jb.46.1.39-56.1943).
- 6 A. Penesyan, I. T. Paulsen, S. Kjelleberg and M. R. Gillings, Three faces of biofilms: a microbial lifestyle, a nascent multicellular organism, and an incubator for diversity, *npj Biofilms Microbiomes*, 2021, **7**(1), 80, DOI: [10.1038/s41522-021-00251-2](https://doi.org/10.1038/s41522-021-00251-2).
- 7 D. Sharma, L. Misba and A. U. Khan, Antibiotics versus biofilm: an emerging battleground in microbial communities, *Antimicrob. Resist. Infect. Control*, 2019, **8**(1), 76, DOI: [10.1186/s13756-019-0533-3](https://doi.org/10.1186/s13756-019-0533-3).
- 8 A. W. Nakawuki, R. Nekaka, L. V. N. Ssenyonga, G. Masifa, D. Nuwasiima and J. Nteziyaremye, *et al.*, Bacterial colonization, species diversity and antimicrobial susceptibility patterns of indwelling urinary catheters from postpartum mothers attending a Tertiary Hospital in Eastern Uganda, *PLoS One*, 2022, **17**(1), e0262414, DOI: [10.1371/journal.pone.0262414](https://doi.org/10.1371/journal.pone.0262414).
- 9 D. van den Berg, D. Asker, T. S. Awad, N. Lavielle and B. D. Hatton, Mechanical deformation of elastomer medical devices can enable microbial surface colonization, *Sci. Rep.*, 2023, **13**(1), 7691, DOI: [10.1038/s41598-023-34217-5](https://doi.org/10.1038/s41598-023-34217-5).
- 10 J. H. Bera, A. L. S. Raj, S. Gang and D. N. Patel, Biofilm, in *Microbial Biofilms*, Elsevier, 2023, pp. 369–390, DOI: [10.1016/B978-0-323-95715-1.00010-8](https://doi.org/10.1016/B978-0-323-95715-1.00010-8).
- 11 V. G. Preda and O. Săndulescu, Communication is the key: biofilms, quorum sensing, formation and prevention, *Discoveries*, 2019, **7**(3), e100, DOI: [10.15190/d.2019.13](https://doi.org/10.15190/d.2019.13), PubMed PMID: 32309618.
- 12 M. Kannan, K. Rajarathinam, S. Venkatesan, B. Dheeba and A. Maniraj, Chapter 19 - Silver Iodide Nanoparticles as an Antibiofilm Agent—A Case Study on Gram-Negative Biofilm-Forming Bacteria, in *Nanostructures for Antimicrobial Therapy*, ed. A. Fica and A. M. Grumezescu, Elsevier, 2017, pp. 435–456, DOI: [10.1016/B978-0-323-46152-8.00019-6](https://doi.org/10.1016/B978-0-323-46152-8.00019-6), Available from: <https://www.sciencedirect.com/science/article/pii/B9780323461528000196>.
- 13 K. Arunasri and S. V. Mohan, Chapter 2.3 - Biofilms: Microbial Life on the Electrode Surface, in *Microbial Electrochemical Technology*, ed. S. V. Mohan, S. Varjani and A. Pandey, Elsevier, 2019, pp. 295–313, DOI: [10.1016/B978-0-444-64052-9.00011-X](https://doi.org/10.1016/B978-0-444-64052-9.00011-X), Available from: <https://www.sciencedirect.com/science/article/pii/B978044464052900011X>.
- 14 P. Shree, C. K. Singh, K. K. Sodhi, J. N. Surya and D. K. Singh, Biofilms: Understanding the structure and contribution towards bacterial resistance in antibiotics, *Med. Microecol.*, 2023, **16**, 100084, DOI: [10.1016/j.medmic.2023.100084](https://doi.org/10.1016/j.medmic.2023.100084).
- 15 A. Zhao, J. Sun and Y. Liu, Understanding bacterial biofilms: From definition to treatment strategies, *Front. Cell. Infect. Microbiol.*, 2023, **13**, 1137947, DOI: [10.3389/fcimb.2023.1137947](https://doi.org/10.3389/fcimb.2023.1137947).
- 16 A. Penesyan, I. T. Paulsen, S. Kjelleberg and M. R. Gillings, Three faces of biofilms: a microbial lifestyle, a nascent multicellular organism, and an incubator for diversity, *npj Biofilms Microbiomes*, 2021, **7**(1), 80, DOI: [10.1038/s41522-021-00251-2](https://doi.org/10.1038/s41522-021-00251-2).
- 17 H. Y. Liu, E. L. Prentice and M. A. Webber, Mechanisms of antimicrobial resistance in biofilms, *npj Antimicrob. Resist.*, 2024, **2**(1), 27, DOI: [10.1038/s44259-024-00046-3](https://doi.org/10.1038/s44259-024-00046-3).
- 18 M. A. Rather, K. Gupta and M. Mandal, Microbial biofilm: formation, architecture, antibiotic resistance, and control strategies, *Braz. J. Microbiol.*, 2021, **52**(4), 1701–1718, DOI: [10.1007/s42770-021-00624-x](https://doi.org/10.1007/s42770-021-00624-x).
- 19 P. N. Danese, Antibiofilm Approaches, *Chem. Biol.*, 2002, **9**(8), 873–880, DOI: [10.1016/S1074-5521\(02\)00192-8](https://doi.org/10.1016/S1074-5521(02)00192-8).
- 20 J. Malheiro and M. Simões, Antimicrobial resistance of biofilms in medical devices, in *Biofilms and Implantable Medical Devices*, Elsevier, 2017, pp. 97–113, DOI: [10.1016/B978-0-08-100382-4.00004-6](https://doi.org/10.1016/B978-0-08-100382-4.00004-6).
- 21 D. López, H. Vlamakis and R. Kolter, Biofilms, *Cold Spring Harbor Perspect. Biol.*, 2010, **2**(7), a000398, DOI: [10.1101/cshperspect.a000398](https://doi.org/10.1101/cshperspect.a000398), PubMed PMID: 20519345.

- 22 L. K. Vestby, T. Grønseth, R. Simm and L. L. Nesse, Bacterial Biofilm and its Role in the Pathogenesis of Disease, *Antibiotics*, 2020, **9**(2), 59, DOI: [10.3390/antibiotics9020059](https://doi.org/10.3390/antibiotics9020059).
- 23 S. Mendhe, A. Badge, S. Ugemuge and D. Chandi, Impact of Biofilms on Chronic Infections and Medical Challenges, *Cureus*, 2023, **15**(11), e48204, DOI: [10.7759/cureus.48204](https://doi.org/10.7759/cureus.48204), PubMed PMID: 38050493.
- 24 A. Mishra, A. Aggarwal and F. Khan, Medical Device-Associated Infections Caused by Biofilm-Forming Microbial Pathogens and Controlling Strategies, *Antibiotics*, 2024, **13**(7), 623, DOI: [10.3390/antibiotics13070623](https://doi.org/10.3390/antibiotics13070623).
- 25 L. K. Vestby, T. Grønseth, R. Simm and L. L. Nesse, Bacterial Biofilm and its Role in the Pathogenesis of Disease, *Antibiotics*, 2020, **9**(2), 59, DOI: [10.3390/antibiotics9020059](https://doi.org/10.3390/antibiotics9020059).
- 26 P. Ebenezer, S. P. S. N. B. S. Kumara, S. W. M. A. I. Senevirathne, L. J. Bray, P. Wangchuk and A. Mathew, *et al.*, Advancements in Antimicrobial Surface Coatings Using Metal/Metaloxide Nanoparticles, Antibiotics, and Phytochemicals, *Nanomaterials*, 2025, **15**(13), 1023, DOI: [10.3390/nano15131023](https://doi.org/10.3390/nano15131023).
- 27 World Health Organisation, Global report on infection prevention and control 2024, World Health Organization, Geneva, 2024, Licence: CCBY-NC-SA 3.0 IGO. 2024. Report.
- 28 N. Bouhrour, P. H. Nibbering and F. Bendali, Medical Device-Associated Biofilm Infections and Multidrug-Resistant Pathogens, *Pathogens*, 2024, **13**(5), 393, DOI: [10.3390/pathogens13050393](https://doi.org/10.3390/pathogens13050393).
- 29 D. Sharma, L. Misba and A. U. Khan, Antibiotics versus biofilm: an emerging battleground in microbial communities, *Antimicrob. Resist. Infect. Control*, 2019, **8**(1), 76, DOI: [10.1186/s13756-019-0533-3](https://doi.org/10.1186/s13756-019-0533-3).
- 30 M. I. Hutchings, A. W. Truman and B. Wilkinson, Antibiotics: past, present and future, *Curr. Opin. Microbiol.*, 2019, **51**, 72–80, DOI: [10.1016/j.mib.2019.10.008](https://doi.org/10.1016/j.mib.2019.10.008).
- 31 A. Baran, A. Kwiatkowska and L. Potocki, Antibiotics and Bacterial Resistance—A Short Story of an Endless Arms Race, *Int. J. Mol. Sci.*, 2023, **24**(6), 5777, DOI: [10.3390/ijms24065777](https://doi.org/10.3390/ijms24065777).
- 32 M. A. Salam, M. Y. Al-Amin, M. T. Salam, J. S. Pawar, N. Akhter and A. A. Rabaan, *et al.*, Antimicrobial Resistance: A Growing Serious Threat for Global Public Health, *Healthc.*, 2023, **11**(13), 1946, DOI: [10.3390/healthcare11131946](https://doi.org/10.3390/healthcare11131946).
- 33 P. Shree, C. K. Singh, K. K. Sodhi, J. N. Surya and D. K. Singh, Biofilms: Understanding the structure and contribution towards bacterial resistance in antibiotics, *Med. Microecol.*, 2023, **16**, 100084, DOI: [10.1016/j.medmic.2023.100084](https://doi.org/10.1016/j.medmic.2023.100084).
- 34 N. K. Rai, A. Ashok and B. R. Akondi, Consequences of chemical impact of disinfectants: safe preventive measures against COVID-19, *Crit. Rev. Toxicol.*, 2020, **50**(6), 513–520, DOI: [10.1080/10408444.2020.1790499](https://doi.org/10.1080/10408444.2020.1790499).
- 35 D. Ghafoor, Z. Khan, A. Khan, D. Ualiyeva and N. Zaman, Excessive use of disinfectants against COVID-19 posing a potential threat to living beings, *Curr. Res. Toxicol.*, 2021, **2**, 159–168, DOI: [10.1016/j.crttox.2021.02.008](https://doi.org/10.1016/j.crttox.2021.02.008).
- 36 N. Musee, P. Ngwenya, L. K. Motaung, K. Moshuhla and P. Nomngongo, Occurrence, effects, and ecological risks of chemicals in sanitizers and disinfectants: A review, *Environ. Chem. Ecotoxicol.*, 2023, **5**, 62–78, DOI: [10.1016/j.enccco.2023.01.003](https://doi.org/10.1016/j.enccco.2023.01.003).
- 37 G. McDonnell and A. D. Russell, Antiseptics and Disinfectants: Activity, Action, and Resistance, *Clin. Microbiol. Rev.*, 1999, **12**(1), 147–179, DOI: [10.1128/CMR.12.1.147](https://doi.org/10.1128/CMR.12.1.147).
- 38 P. Pereira-Silva, J. Borges and P. Sampaio, Recent advances in metal-based antimicrobial coatings, *Adv. Colloid Interface Sci.*, 2025, **344**, 103590, DOI: [10.1016/j.cis.2025.103590](https://doi.org/10.1016/j.cis.2025.103590).
- 39 M. Birkett, L. Dover, C. Cherian Lukose, A. Wasy Zia, M. M. Tambuwala and Á. Serrano-Aroca, Recent Advances in Metal-Based Antimicrobial Coatings for High-Touch Surfaces, *Int. J. Mol. Sci.*, 2022, **23**(3), 1162, DOI: [10.3390/ijms23031162](https://doi.org/10.3390/ijms23031162).
- 40 R. F. Hamarawf, Antibacterial, antibiofilm, and antioxidant activities of two novel metal–organic frameworks (MOFs) based on 4,6-diamino-2-pyrimidinethiol with Zn and Co metal ions as coordination polymers, *RSC Adv.*, 2024, **14**(13), 9080–9098, DOI: [10.1039/D4RA00545G](https://doi.org/10.1039/D4RA00545G).
- 41 R. Huang, Z. Zhou, X. Lan, F. K. Tang, T. Cheng and H. Sun, *et al.*, Rapid synthesis of bismuth-organic frameworks as selective antimicrobial materials against microbial biofilms, *Mater. Today Bio*, 2023, **18**, 100507, DOI: [10.1016/j.mtbio.2022.100507](https://doi.org/10.1016/j.mtbio.2022.100507).
- 42 M. M. Sabzehmeidani and M. Kazemzad, Recent advances in surface-mounted metal–organic framework thin film coatings for biomaterials and medical applications: a review, *Biomater. Res.*, 2023, **27**, 115, DOI: [10.1186/s40824-023-00454-y](https://doi.org/10.1186/s40824-023-00454-y).
- 43 M. Rai, A. Yadav and A. Gade, Silver nanoparticles as a new generation of antimicrobials, *Biotechnol. Adv.*, 2009, **27**(1), 76–83, DOI: [10.1016/j.biotechadv.2008.09.002](https://doi.org/10.1016/j.biotechadv.2008.09.002).
- 44 S. Dwivedi, R. Wahab, F. Khan, Y. K. Mishra, J. Musarrat and A. A. Al-Khedhairi, Reactive Oxygen Species Mediated Bacterial Biofilm Inhibition via Zinc Oxide Nanoparticles and Their Statistical Determination, *PLoS One*, 2014, **9**(11), e111289, DOI: [10.1371/journal.pone.0111289](https://doi.org/10.1371/journal.pone.0111289).
- 45 I. Salah, I. P. Parkin and E. Allan, Copper as an antimicrobial agent: recent advances, *RSC Adv.*, 2021, **11**(30), 18179–18186, DOI: [10.1039/D1RA02149D](https://doi.org/10.1039/D1RA02149D).
- 46 N. Bisht, N. Dwivedi, P. Kumar, M. Venkatesh, A. K. Yadav and D. Mishra, *et al.*, Recent advances in copper and copper-derived materials for antimicrobial resistance and infection control, *Curr. Opin. Biomed. Eng.*, 2022, **24**, 100408, DOI: [10.1016/j.cobme.2022.100408](https://doi.org/10.1016/j.cobme.2022.100408).
- 47 X. Liu and M. Kamperman, Smart bacteria-responsive coatings for combating catheter-associated urinary tract infections, *Mater. Today Bio*, 2025, **34**, 102191, DOI: [10.1016/j.mtbio.2025.102191](https://doi.org/10.1016/j.mtbio.2025.102191).
- 48 S. D. Morgan, D. Rigby and D. J. Stickler, A study of the structure of the crystalline bacterial biofilms that can encrust and block silver Foley catheters, *Urol. Res.*, 2009, **37**(2), 89–93, DOI: [10.1007/s00240-009-0176-6](https://doi.org/10.1007/s00240-009-0176-6).
- 49 R. M. Ortí-Lucas and J. Muñoz-Miguel, Effectiveness of surface coatings containing silver ions in bacterial

- decontamination in a recovery unit, *Antimicrob. Resist. Infect. Control*, 2017, **6**(1), 61, DOI: [10.1186/s13756-017-0217-9](https://doi.org/10.1186/s13756-017-0217-9).
- 50 C. Wang, X. Wei, L. Zhong, C. L. Chan, H. Li and H. Sun, Metal-Based Approaches for the Fight against Antimicrobial Resistance: Mechanisms, Opportunities, and Challenges, *J. Am. Chem. Soc.*, 2025, **147**(15), 12361–12380, DOI: [10.1021/jacs.4c16035](https://doi.org/10.1021/jacs.4c16035).
 - 51 X. t. Shen, Y. z. Zhang, F. Xiao, J. Zhu and X. Zheng, Effects on cytotoxicity and antibacterial properties of the incorporations of silver nanoparticles into the surface coating of dental alloys, *J. Zhejiang Univ., Sci., B*, 2017, **18**(7), 615–625, DOI: [10.1631/jzus.B1600555](https://doi.org/10.1631/jzus.B1600555).
 - 52 J. Y. Maillard and M. Pascoe, Disinfectants and antiseptics: mechanisms of action and resistance, *Nat. Rev. Microbiol.*, 2024, **22**(1), 4–17, DOI: [10.1038/s41579-023-00958-3](https://doi.org/10.1038/s41579-023-00958-3).
 - 53 C. Nunez, R. S. Bamert, K. Lambert and F. L. Short, Cleaning up our disinfectants: usage of antimicrobial biocides in direct-to-consumer products in Australia, *Access Microbiol.*, 2024, **6**(2), 000714.v3, DOI: [10.1099/acmi.0.000714.v3](https://doi.org/10.1099/acmi.0.000714.v3).
 - 54 J. L. Graves, Microbial defense, in *Principles and Applications of Antimicrobial Nanomaterials*, Elsevier, 2022, pp. 137–159, DOI: [10.1016/B978-0-12-822105-1.00017-2](https://doi.org/10.1016/B978-0-12-822105-1.00017-2).
 - 55 D. I. Andersson and D. Hughes, Antibiotic resistance and its cost: is it possible to reverse resistance?, *Nat. Rev. Microbiol.*, 2010, **8**(4), 260–271, DOI: [10.1038/nrmicro2319](https://doi.org/10.1038/nrmicro2319).
 - 56 J. O'Neill, Antimicrobial resistance : tackling a crisis for the health and wealth of nations/the Review on Antimicrobial Resistance chaired by Jim O'Neill. Attribution 4.0 International (CC BY 4.0), Source: Wellcome Collection, 2014.
 - 57 M. A. Salam, M. Y. Al-Amin, M. T. Salam, J. S. Pawar, N. Akhter and A. A. Rabaan, *et al.*, Antimicrobial Resistance: A Growing Serious Threat for Global Public Health, *Healthc.*, 2023, **11**(13), 1946, DOI: [10.3390/healthcare11131946](https://doi.org/10.3390/healthcare11131946).
 - 58 C. J. L. Murray, K. S. Ikuta, F. Sharara, L. Swetschinski, G. Robles Aguilar and A. Gray, *et al.*, Global burden of bacterial antimicrobial resistance in 2019: a systematic analysis, *Lancet*, 2022, **399**(10325), 629–655, DOI: [10.1016/S0140-6736\(21\)02724-0](https://doi.org/10.1016/S0140-6736(21)02724-0).
 - 59 U. Mahanta, M. Khandelwal and A. S. Deshpande, Antimicrobial surfaces: a review of synthetic approaches, applicability and outlook, *J. Mater. Sci.*, 2021, **56**(32), 17915–17941, DOI: [10.1007/s10853-021-06404-0](https://doi.org/10.1007/s10853-021-06404-0).
 - 60 M. Sheridan, C. Winters, F. Zamboni and M. N. Collins, Biomaterials: Antimicrobial surfaces in biomedical engineering and healthcare, *Curr. Opin. Biomed. Eng.*, 2022, **22**, 100373, DOI: [10.1016/j.cobme.2022.100373](https://doi.org/10.1016/j.cobme.2022.100373).
 - 61 Q. Su, Y. Xue, C. Wang, Q. Zhou, Y. Zhao and J. Su, *et al.*, Strategies and applications of antibacterial surface-modified biomaterials, *Bioact. Mater.*, 2025, **53**, 114–140, DOI: [10.1016/j.bioactmat.2025.07.009](https://doi.org/10.1016/j.bioactmat.2025.07.009).
 - 62 S. Fernandes, I. B. Gomes, M. Simões and L. C. Simões, Novel chemical-based approaches for biofilm cleaning and disinfection, *Curr. Opin. Food Sci.*, 2024, **55**, 101124, DOI: [10.1016/j.cofs.2024.101124](https://doi.org/10.1016/j.cofs.2024.101124).
 - 63 K. K. Chung, J. F. Schumacher, E. M. Sampson, R. A. Burne, P. J. Antonelli and A. B. Brennan, Impact of engineered surface microtopography on biofilm formation of *Staphylococcus aureus*, *Biointerphases*, 2007, **2**(2), 89–94, DOI: [10.1116/1.2751405](https://doi.org/10.1116/1.2751405).
 - 64 J. C. Tiller, C. J. Liao, K. Lewis and A. M. Klibanov, Designing surfaces that kill bacteria on contact, *Proc. Natl. Acad. Sci. U. S. A.*, 2001, **98**(11), 5981–5985, DOI: [10.1073/pnas.111143098](https://doi.org/10.1073/pnas.111143098).
 - 65 E. P. Ivanova, V. K. Truong, H. K. Webb, V. A. Baulin, J. Y. Wang and N. Mohammadi, *et al.*, Differential attraction and repulsion of *Staphylococcus aureus* and *Pseudomonas aeruginosa* on molecularly smooth titanium films, *Sci. Rep.*, 2011, **1**(1), 165, DOI: [10.1038/srep00165](https://doi.org/10.1038/srep00165).
 - 66 B. Mrabet, M. N. Nguyen, A. Majbri, S. Mahouche, M. Turmine and A. Bakhrouf, *et al.*, Anti-fouling poly(2-hydroxyethyl methacrylate) surface coatings with specific bacteria recognition capabilities, *Surf. Sci.*, 2009, **603**(16), 2422–2429, DOI: [10.1016/j.susc.2009.05.020](https://doi.org/10.1016/j.susc.2009.05.020).
 - 67 E. P. Ivanova, J. Hasan, H. K. Webb, V. K. Truong, G. S. Watson and J. A. Watson, *et al.*, Natural Bactericidal Surfaces: Mechanical Rupture of *Pseudomonas aeruginosa* Cells by Cicada Wings, *Small*, 2012, **8**(16), 2489–2494, DOI: [10.1002/sml.201200528](https://doi.org/10.1002/sml.201200528).
 - 68 A. Elbourne, R. J. Crawford and E. P. Ivanova, Nano-structured antimicrobial surfaces: From nature to synthetic analogues, *J. Colloid Interface Sci.*, 2017, **508**, 603–616, DOI: [10.1016/j.jcis.2017.07.021](https://doi.org/10.1016/j.jcis.2017.07.021).
 - 69 W. Barthlott and C. Neinhuis, Purity of the sacred lotus, or escape from contamination in biological surfaces, *Planta*, 1997, **202**(1), 1–8, DOI: [10.1007/s004250050096](https://doi.org/10.1007/s004250050096).
 - 70 E. P. Ivanova, J. Hasan, H. K. Webb, V. K. Truong, G. S. Watson and J. A. Watson, *et al.*, Natural Bactericidal Surfaces: Mechanical Rupture of *Pseudomonas aeruginosa* Cells by Cicada Wings, *Small*, 2012, **8**(16), 2489–2494, DOI: [10.1002/sml.201200528](https://doi.org/10.1002/sml.201200528).
 - 71 K. Liu and L. Jiang, Bio-inspired design of multiscale structures for function integration, *Nano Today*, 2011, **6**(2), 155–175, DOI: [10.1016/j.nantod.2011.02.002](https://doi.org/10.1016/j.nantod.2011.02.002).
 - 72 A. Velic, J. Hasan, Z. Li and P. K. D. V. Yarlagadda, Mechanics of Bacterial Interaction and Death on Nanopatterned Surfaces, *Biophys. J.*, 2021, **120**(2), 217–231, DOI: [10.1016/j.bpj.2020.12.003](https://doi.org/10.1016/j.bpj.2020.12.003).
 - 73 H. W. Chien, X. Y. Chen, W. P. Tsai and M. Lee, Inhibition of biofilm formation by rough shark skin-patterned surfaces, *Colloids Surf., B*, 2020, **186**, 110738, DOI: [10.1016/j.colsurfb.2019.110738](https://doi.org/10.1016/j.colsurfb.2019.110738).
 - 74 G. Tian, D. Fan, X. Feng and H. Zhou, Thriving artificial underwater drag-reduction materials inspired from aquatic animals: progresses and challenges, *RSC Adv.*, 2021, **11**(6), 3399–3428, DOI: [10.1039/D0RA08672J](https://doi.org/10.1039/D0RA08672J).
 - 75 E. E. Mann, D. Manna, M. R. Mettetal, R. M. May, E. M. Dannemiller and K. K. Chung, *et al.*, Surface micropattern limits bacterial contamination, *Antimicrob. Resist. Infect. Control*, 2014, **3**(1), 28, DOI: [10.1186/2047-2994-3-28](https://doi.org/10.1186/2047-2994-3-28).

- 76 Q. Liu, L. Brookbank, A. Ho, J. Coffey, A. B. Brennan and C. J. Jones, Surface texture limits transfer of *S. aureus*, T4 Bacteriophage, Influenza B virus and Human coronavirus, *PLoS One*, 2020, **15**(12), e0244518, DOI: [10.1371/journal.pone.0244518](https://doi.org/10.1371/journal.pone.0244518).
- 77 S. T. Reddy, K. K. Chung, C. J. McDaniel, R. O. Darouiche, J. Landman and A. B. Brennan, Micropatterned Surfaces for Reducing the Risk of Catheter-Associated Urinary Tract Infection: An *In Vitro* Study on the Effect of Sharklet Micropatterned Surfaces to Inhibit Bacterial Colonization and Migration of Uropathogenic *Escherichia coli*, *J. Endourol.*, 2011, **25**(9), 1547–1552, DOI: [10.1089/end.2010.0611](https://doi.org/10.1089/end.2010.0611).
- 78 S. Arango-Santander, Bioinspired Topographic Surface Modification of Biomaterials, *Materials*, 2022, **15**(7), 2383, DOI: [10.3390/ma15072383](https://doi.org/10.3390/ma15072383).
- 79 J. Redfern, A. J. Cunliffe, D. M. Goeres, N. F. Azevedo and J. Verran, Critical analysis of methods to determine growth, control and analysis of biofilms for potential non-submerged antibiofilm surfaces and coatings, *Biofilm*, 2024, **7**, 100187, DOI: [10.1016/j.biofilm.2024.100187](https://doi.org/10.1016/j.biofilm.2024.100187).
- 80 L. Li, N. Mendis, H. Trigui, J. D. Oliver and S. P. Faucher, The importance of the viable but non-culturable state in human bacterial pathogens, *Front. Microbiol.*, 2014, **5**, 258, DOI: [10.3389/fmicb.2014.00258](https://doi.org/10.3389/fmicb.2014.00258).
- 81 E. Haney, M. Trimble, J. Cheng, Q. Vallé and R. Hancock, Critical Assessment of Methods to Quantify Biofilm Growth and Evaluate Antibiofilm Activity of Host Defence Peptides, *Biomolecules*, 2018, **8**(2), 29, DOI: [10.3390/biom8020029](https://doi.org/10.3390/biom8020029).
- 82 C. T. Meyer, G. K. Lynch, D. F. Stamo, E. J. Miller, A. Chatterjee and J. M. Kralj, A high-throughput and low-waste viability assay for microbes, *Nat. Microbiol.*, 2023, **8**(12), 2304–2314, DOI: [10.1038/s41564-023-01513-9](https://doi.org/10.1038/s41564-023-01513-9).
- 83 K. M. Martini, S. S. Boddu, I. Nemenman and N. M. Vega, Maximum likelihood estimators for colony-forming units, *Microbiol. Spectrum*, 2024, **12**(9), 1–17, DOI: [10.1128/spectrum.03946-23](https://doi.org/10.1128/spectrum.03946-23).
- 84 D. Gerardi, S. Bernardi, A. Bruni, G. Falisi and G. Botticelli, Characterization and morphological methods for oral biofilm visualization: where are we nowadays?, *AIMS Microbiol.*, 2024, **10**(2), 391–414, DOI: [10.3934/microbiol.2024020](https://doi.org/10.3934/microbiol.2024020).
- 85 A. A. Awadh, A. F. Kelly, G. Forster-Wilkins, D. Wertheim, R. Giddens and S. W. Gould, *et al.*, Visualisation and biovolume quantification in the characterisation of biofilm formation in *Mycoplasma fermentans*, *Sci. Rep.*, 2021, **11**(1), 11259, DOI: [10.1038/s41598-021-90455-5](https://doi.org/10.1038/s41598-021-90455-5).
- 86 T. Nishida, S. Seino and Y. Imoto, Visualizing Antimicrobial Effects on Bacterial Surfaces by <sc>SEM</sc> : A Comparative Study of Hexamethyldisilazane (<sc>HMDS</sc>) and Freeze-Drying, *Microsc. Res. Tech.*, 2025, **88**(12), 3273–3281, DOI: [10.1002/jemt.70037](https://doi.org/10.1002/jemt.70037).
- 87 M. Rosenberg, N. F. Azevedo and A. Ivask, Propidium iodide staining underestimates viability of adherent bacterial cells, *Sci. Rep.*, 2019, **9**(1), 6483, DOI: [10.1038/s41598-019-42906-3](https://doi.org/10.1038/s41598-019-42906-3).
- 88 P. Stiefel, S. Schmidt-Emrich, K. Maniura-Weber and Q. Ren, Critical aspects of using bacterial cell viability assays with the fluorophores SYTO9 and propidium iodide, *BMC Microbiol.*, 2015, **15**(1), 36, DOI: [10.1186/s12866-015-0376-x](https://doi.org/10.1186/s12866-015-0376-x).
- 89 T. Tchatchiashvili, M. Jundzill, M. Marquet, K. A. Mirza, M. W. Pletz and O. Makarewicz, *et al.*, CAM/TMA-DPH as a promising alternative to SYTO9/PI for cell viability assessment in bacterial biofilms, *Front. Cell. Infect. Microbiol.*, 2025, **14**, 1–13, DOI: [10.3389/fcimb.2024.1508016](https://doi.org/10.3389/fcimb.2024.1508016).
- 90 L. Netuschil, T. M. Auschill, A. Sculean and N. B. Arweiler, Confusion over live/dead stainings for the detection of vital microorganisms in oral biofilms - which stain is suitable?, *BMC Oral Health*, 2014, **14**(1), 2, DOI: [10.1186/1472-6831-14-2](https://doi.org/10.1186/1472-6831-14-2).
- 91 N. Raab and I. Bachelet, Resolving biofilm topography by native scanning electron microscopy, *J. Biol. Methods*, 2024, **4**(2), 1, DOI: [10.14440/jbm.2017.173](https://doi.org/10.14440/jbm.2017.173).
- 92 M. Kumar and R. Bhardwaj, Wetting characteristics of *Colocasia esculenta* (Taro) leaf and a bioinspired surface thereof, *Sci. Rep.*, 2020, **10**(1), 935, DOI: [10.1038/s41598-020-57410-2](https://doi.org/10.1038/s41598-020-57410-2).
- 93 N. Cates, V. J. Einck, L. Micklow, J. Morère, U. Okoroanyanwu and J. J. Watkins, *et al.*, Roll-to-roll nanoimprint lithography using a seamless cylindrical mold nanopatterned with a high-speed mastering process, *Nanotechnology*, 2021, **32**(15), 155301, DOI: [10.1088/1361-6528/abd9f1](https://doi.org/10.1088/1361-6528/abd9f1).
- 94 N. Kooy, K. Mohamed, L. T. Pin and O. S. Guan, A review of roll-to-roll nanoimprint lithography, *Nanoscale Res. Lett.*, 2014, **9**(1), 320, DOI: [10.1186/1556-276X-9-320](https://doi.org/10.1186/1556-276X-9-320).
- 95 F. Dundar Arisoy, K. W. Kolewe, B. Homyak, I. S. Kurtz, J. D. Schiffman and J. J. Watkins, Bioinspired Photocatalytic Shark-Skin Surfaces with Antibacterial and Antifouling Activity via Nanoimprint Lithography, *ACS Appl. Mater. Interfaces*, 2018, **10**(23), 20055–20063, DOI: [10.1021/acsami.8b05066](https://doi.org/10.1021/acsami.8b05066).
- 96 C. Du, C. Wang, T. Zhang and L. Zheng, Antibacterial Performance of Zr-BMG, Stainless Steel, and Titanium Alloy with Laser-Induced Periodic Surface Structures, *ACS Appl. Bio Mater.*, 2022, **5**(1), 272–284, DOI: [10.1021/acsabm.1c01075](https://doi.org/10.1021/acsabm.1c01075).
- 97 J. Bonse, S. V. Kirner and J. Krüger, Laser-Induced Periodic Surface Structures (LIPSS), in *Handbook of Laser Micro- and Nano-Engineering*, ed. K. Sugioka, Springer International Publishing, Cham, 2020, pp. 1–59, DOI: [10.1007/978-3-319-69537-2_17-1](https://doi.org/10.1007/978-3-319-69537-2_17-1).
- 98 S. Grossmann, L. Tetzlaff, N. Grabow, K. P. Schmitz and S. Siewert, LIPSS on polymeric implant surfaces - a fabrication study, *Curr. Dir. Biomed. Eng.*, 2024, **10**(4), 280–283, DOI: [10.1515/cdbme-2024-2068](https://doi.org/10.1515/cdbme-2024-2068).
- 99 R. Gupta, A. Gaddam, D. Prajapati, S. Dimov, A. Mishra and M. Vadali, Enhancing Bactericidal Properties of Ti6Al4V Surfaces through Micro and Nano Hierarchical Laser Texturing, *Langmuir*, 2024, **40**(32), 16791–16803, DOI: [10.1021/acs.langmuir.4c01173](https://doi.org/10.1021/acs.langmuir.4c01173).
- 100 K. Oubellaouch, L. Orazi, P. Brun, G. Lucchetta, R. Pelaccia and M. Sorgato, An innovative process chain for the

- production of antibiofouling polymer parts using ultrafast laser texturing, *Int. J. Adv. Des. Manuf. Technol.*, 2024, **134**, 3653–3664, DOI: [10.1007/s00170-024-14369-y](https://doi.org/10.1007/s00170-024-14369-y).
- 101 N. Lozano-Hernández, G. Pérez Llanos, C. Saez Comet, L. J. del Valle, J. Puiggali and E. Fontdecaba, Micro- and Nanotexturization of Liquid Silicone Rubber Surfaces by Injection Molding Using Hybrid Polymer Inlays, *Macromol. Mater. Eng.*, 2022, **307**, 2100741, DOI: [10.1002/mame.202100741](https://doi.org/10.1002/mame.202100741).
 - 102 A. Jaggesar, H. Shahali, A. Mathew and P. K. D. V. Yarlagadda, Bio-mimicking nano and micro-structured surface fabrication for antibacterial properties in medical implants, *J. Nanobiotechnol.*, 2017, **15**(1), 64, DOI: [10.1186/s12951-017-0306-1](https://doi.org/10.1186/s12951-017-0306-1).
 - 103 S. K. Yadav, S. Aravindan and P. V. Rao, Characterisation of micro-textures created by hot embossing on polystyrene for probable use as an antireflective coating, *Surf. Eng.*, 2025, **41**(3), 403–416, DOI: [10.1177/02670844251321586](https://doi.org/10.1177/02670844251321586).
 - 104 E. P. Ivanova, J. Hasan, H. K. Webb, G. Gervinskas, S. Juodkazis and V. K. Truong, *et al.*, Bactericidal activity of black silicon, *Nat. Commun.*, 2013, **4**(1), 2838, DOI: [10.1038/ncomms3838](https://doi.org/10.1038/ncomms3838).
 - 105 M. Benčina, M. Resnik, P. Starič and I. Junkar, Use of Plasma Technologies for Antibacterial Surface Properties of Metals, *Molecules*, 2021, **26**(5), 1418, DOI: [10.3390/molecules26051418](https://doi.org/10.3390/molecules26051418).
 - 106 M. Asadi Tokmedash, C. Kim, A. P. Chavda, A. Li, J. Robins and J. Min, Engineering multifunctional surface topography to regulate multiple biological responses, *Biomaterials*, 2025, **319**, 123136, DOI: [10.1016/j.biomaterials.2025.123136](https://doi.org/10.1016/j.biomaterials.2025.123136).
 - 107 F. Yang, Z. Pan, L. Shen, D. Huang, H. Gao and X. Wang, *et al.*, Recent advances in marine biomimetic antifouling technology based on microstructured surfaces inspired by aquatic organisms, *J. Coat. Technol. Res.*, 2026, 1–20, DOI: [10.1007/s11998-025-01219-z](https://doi.org/10.1007/s11998-025-01219-z).
 - 108 A. Francone, S. Merino, A. Retolaza, J. Ramiro, S. A. Alves and J. V. de Castro, *et al.*, Impact of surface topography on the bacterial attachment to micro- and nano-patterned polymer films, *Surf. Interfaces*, 2021, **27**, 101494, DOI: [10.1016/j.surf.2021.101494](https://doi.org/10.1016/j.surf.2021.101494).
 - 109 M. I. Ishak, X. Liu, J. Jenkins, A. H. Nobbs and B. Su, Protruding Nanostructured Surfaces for Antimicrobial and Osteogenic Titanium Implants, *Coatings*, 2020, **10**(8), 756, DOI: [10.3390/coatings10080756](https://doi.org/10.3390/coatings10080756).
 - 110 R. Jiang, L. Hao, L. Song, L. Tian, Y. Fan and J. Zhao, *et al.*, Lotus-leaf-inspired hierarchical structured surface with non-fouling and mechanical bactericidal performances, *Chem. Eng. J.*, 2020, **398**, 125609, DOI: [10.1016/j.cej.2020.125609](https://doi.org/10.1016/j.cej.2020.125609).
 - 111 J. A. Moran, B. J. Hawkins, B. E. Gowen and S. L. Robbins, Ion fluxes across the pitcher walls of three Bornean Nepenthes pitcher plant species: flux rates and gland distribution patterns reflect nitrogen sequestration strategies, *J. Exp. Bot.*, 2010, **61**(5), 1365–1374, DOI: [10.1093/jxb/erq004](https://doi.org/10.1093/jxb/erq004).
 - 112 B. P. Kamarajan and A. Muthusamy, Survival strategy of *Pseudomonas aeruginosa* on the nanopillar topography of dragonfly (*Pantala flavescens*) wing, *AMB Express*, 2020, **10**(1), 85, DOI: [10.1186/s13568-020-01021-7](https://doi.org/10.1186/s13568-020-01021-7).
 - 113 S. Pogodin, J. Hasan, V. A. Baulin, H. K. Webb, V. K. Truong and T. H. Phong Nguyen, *et al.*, Biophysical Model of Bacterial Cell Interactions with Nanopatterned Cicada Wing Surfaces, *Biophys. J.*, 2013, **104**(4), 835–840, DOI: [10.1016/j.bpj.2012.12.046](https://doi.org/10.1016/j.bpj.2012.12.046).
 - 114 G. S. Watson, D. W. Green, L. Schwarzkopf, X. Li, B. W. Cribb and S. Myhra, *et al.*, A gecko skin micro/nano structure – A low adhesion, superhydrophobic, anti-wetting, self-cleaning, biocompatible, antibacterial surface, *Acta Biomater.*, 2015, **21**, 109–122, DOI: [10.1016/j.actbio.2015.03.007](https://doi.org/10.1016/j.actbio.2015.03.007).
 - 115 M. Yang, Y. Ding, X. Ge and Y. Leng, Control of bacterial adhesion and growth on honeycomb-like patterned surfaces, *Colloids Surf., B*, 2015, **135**, 549–555, DOI: [10.1016/j.colsurfb.2015.08.010](https://doi.org/10.1016/j.colsurfb.2015.08.010).
 - 116 A. Elbourne, V. E. Coyle, V. K. Truong, Y. M. Sabri, A. E. Kandjani and S. K. Bhargava, *et al.*, Multi-directional electrodeposited gold nanospikes for antibacterial surface applications, *Nanoscale Adv.*, 2019, **1**(1), 203–212, DOI: [10.1039/C8NA00124C](https://doi.org/10.1039/C8NA00124C).
 - 117 A. Khursheed, L. Xu and C. A. Siedlecki, The effects of submicron-textured surface topography on antibiotic efficacy against biofilms, *J. Biomed. Mater. Res., Part B*, 2024, **112**(7), 1–24, DOI: [10.1002/jbm.b.35436](https://doi.org/10.1002/jbm.b.35436).
 - 118 A. Singh and E. S. Yoon, Biomimetics in Tribology - Recent Developments, *J. Korean Phys. Soc.*, 2008, **52**(3), 656–668, DOI: [10.3938/jkps.52.656](https://doi.org/10.3938/jkps.52.656).
 - 119 S. Latthe, C. Terashima, K. Nakata and A. Fujishima, Superhydrophobic Surfaces Developed by Mimicking Hierarchical Surface Morphology of Lotus Leaf, *Molecules*, 2014, **19**(4), 4256–4283, DOI: [10.3390/molecules19044256](https://doi.org/10.3390/molecules19044256).
 - 120 A. Zhao, J. Sun and Y. Liu, Understanding bacterial biofilms: From definition to treatment strategies, *Front. Cell. Infect. Microbiol.*, 2023, **13**, 1–23, DOI: [10.3389/fcimb.2023.1137947](https://doi.org/10.3389/fcimb.2023.1137947).
 - 121 J. Ma, Y. Sun, K. Gleichauf, J. Lou and Q. Li, Nanostructure on Taro Leaves Resists Fouling by Colloids and Bacteria under Submerged Conditions, *Langmuir*, 2011, **27**(16), 10035–10040, DOI: [10.1021/la2010024](https://doi.org/10.1021/la2010024).
 - 122 F. H. Rajab, C. M. Liauw, P. S. Benson, L. Li and K. A. Whitehead, Production of hybrid macro/micro/nano surface structures on Ti6Al4V surfaces by picosecond laser surface texturing and their antifouling characteristics, *Colloids Surf., B*, 2017, **160**, 688–696, DOI: [10.1016/j.colsurfb.2017.10.008](https://doi.org/10.1016/j.colsurfb.2017.10.008).
 - 123 M. V. Ankheily, D. K. Wainwright and G. V. Lauder, Diversity of dermal denticle structure in sharks: Skin surface roughness and three-dimensional morphology, *J. Morphol.*, 2018, **279**(8), 1132–1154, DOI: [10.1002/jmor.20836](https://doi.org/10.1002/jmor.20836).
 - 124 S. M. Kelleher, O. Habimana, J. Lawler, B. O'Reilly, S. Daniels and E. Casey, *et al.*, Cicada Wing Surface Topography: An Investigation into the Bactericidal Properties of Nanostructural Features, *ACS Appl. Mater. Interfaces*, 2016, **8**(24), 14966–14974, DOI: [10.1021/acsami.5b08309](https://doi.org/10.1021/acsami.5b08309).

- 125 S. M. Kelleher, O. Habimana, J. Lawler, B. O'Reilly, S. Daniels and E. Casey, *et al.*, Cicada Wing Surface Topography: An Investigation into the Bactericidal Properties of Nanostructural Features, *ACS Appl. Mater. Interfaces*, 2016, **8**(24), 14966–14974, DOI: [10.1021/acsami.5b08309](https://doi.org/10.1021/acsami.5b08309).
- 126 E. P. Ivanova, J. Hasan, H. K. Webb, G. Gervinskas, S. Juodkazis and V. K. Truong, *et al.*, Bactericidal activity of black silicon, *Nat. Commun.*, 2013, **4**(1), 2838, DOI: [10.1038/ncomms3838](https://doi.org/10.1038/ncomms3838).
- 127 C. D. Bandara, S. Singh, I. O. Afara, A. Wolff, T. Tesfamichael and K. Ostrikov, *et al.*, Bactericidal Effects of Natural Nanotopography of Dragonfly Wing on *Escherichia coli*, *ACS Appl. Mater. Interfaces*, 2017, **9**(8), 6746–6760, DOI: [10.1021/acsami.6b13666](https://doi.org/10.1021/acsami.6b13666).
- 128 D. E. Mainwaring, S. H. Nguyen, H. Webb, T. Jakubov, M. Tobin and R. N. Lamb, *et al.*, The nature of inherent bactericidal activity: insights from the nanotopology of three species of dragonfly, *Nanoscale*, 2016, **8**(12), 6527–6534, DOI: [10.1039/C5NR08542J](https://doi.org/10.1039/C5NR08542J).
- 129 D. P. Linklater, S. Juodkazis, R. J. Crawford and E. P. Ivanova, Mechanical inactivation of *Staphylococcus aureus* and *Pseudomonas aeruginosa* by titanium substrata with hierarchical surface structures, *Materialia*, 2019, **5**, 100197, DOI: [10.1016/j.mtla.2018.100197](https://doi.org/10.1016/j.mtla.2018.100197).
- 130 W. Li, E. S. Thian, M. Wang, Z. Wang and L. Ren, Surface Design for Antibacterial Materials: From Fundamentals to Advanced Strategies, *Adv. Sci.*, 2021, **8**(19), 1–23, DOI: [10.1002/advs.202100368](https://doi.org/10.1002/advs.202100368).
- 131 V. K. Truong, N. M. Geeganagamage, V. A. Baulin, J. Vongsivut, M. J. Tobin and P. Luque, *et al.*, The susceptibility of *Staphylococcus aureus* CIP 65.8 and *Pseudomonas aeruginosa* ATCC 9721 cells to the bactericidal action of nanostructured *Calopteryx haemorrhoidalis* damselfly wing surfaces, *Appl. Microbiol. Biotechnol.*, 2017, **101**(11), 4683–4690, DOI: [10.1007/s00253-017-8205-9](https://doi.org/10.1007/s00253-017-8205-9).
- 132 D. P. Linklater, V. A. Baulin, X. Le Guével, J. Fleury, E. Hanssen and T. H. P. Nguyen, *et al.*, Antibacterial Action of Nanoparticles by Lethal Stretching of Bacterial Cell Membranes, *Adv. Mater.*, 2020, **32**(52), 1–15, DOI: [10.1002/adma.202005679](https://doi.org/10.1002/adma.202005679).
- 133 G. Hazell, P. W. May, P. Taylor, A. H. Nobbs, C. C. Welch and B. Su, Studies of black silicon and black diamond as materials for antibacterial surfaces, *Biomater. Sci.*, 2018, **6**(6), 1424–1432, DOI: [10.1039/C8BM00107C](https://doi.org/10.1039/C8BM00107C).
- 134 K. Modaresifar, S. Azizian, M. Ganjian, L. E. Fratila-Apachitei and A. A. Zadpoor, Bactericidal effects of nanopatterns: A systematic review, *Acta Biomater.*, 2019, **83**, 29–36, DOI: [10.1016/j.actbio.2018.09.059](https://doi.org/10.1016/j.actbio.2018.09.059).
- 135 E. P. Ivanova, J. Hasan, H. K. Webb, G. Gervinskas, S. Juodkazis and V. K. Truong, *et al.*, Bactericidal activity of black silicon, *Nat. Commun.*, 2013, **4**(1), 2838, DOI: [10.1038/ncomms3838](https://doi.org/10.1038/ncomms3838).
- 136 M. Mu, S. Liu, W. DeFlorio, L. Hao, X. Wang and K. S. Salazar, *et al.*, Influence of Surface Roughness, Nanostructure, and Wetting on Bacterial Adhesion, *Langmuir*, 2023, **39**(15), 5426–5439, DOI: [10.1021/acs.langmuir.3c00091](https://doi.org/10.1021/acs.langmuir.3c00091).
- 137 D. Perera-Costa, J. M. Bruque, M. L. González-Martín, A. C. Gómez-García and V. Vadillo-Rodríguez, Studying the Influence of Surface Topography on Bacterial Adhesion using Spatially Organized Microtopographic Surface Patterns, *Langmuir*, 2014, **30**(16), 4633–4641, DOI: [10.1021/la5001057](https://doi.org/10.1021/la5001057).
- 138 M. Mu, S. Liu, W. DeFlorio, L. Hao, X. Wang and K. S. Salazar, *et al.*, Influence of Surface Roughness, Nanostructure, and Wetting on Bacterial Adhesion, *Langmuir*, 2023, **39**(15), 5426–5439, DOI: [10.1021/acs.langmuir.3c00091](https://doi.org/10.1021/acs.langmuir.3c00091).
- 139 A. Tripathy, P. Sen, B. Su and W. H. Briscoe, Natural and bioinspired nanostructured bactericidal surfaces, *Adv. Colloid Interface Sci.*, 2017, **248**, 85–104, DOI: [10.1016/j.cis.2017.07.030](https://doi.org/10.1016/j.cis.2017.07.030).
- 140 J. Hasan, S. Raj, L. Yadav and K. Chatterjee, Engineering a nanostructured “super surface” with superhydrophobic and superkilling properties, *RSC Adv.*, 2015, **5**(56), 44953–44959, DOI: [10.1039/C5RA05206H](https://doi.org/10.1039/C5RA05206H).
- 141 D. P. Linklater, H. K. D. Nguyen, C. M. Bhadra, S. Juodkazis and E. P. Ivanova, Influence of nanoscale topology on bactericidal efficiency of black silicon surfaces, *Nanotechnology*, 2017, **28**(24), 245301, DOI: [10.1088/1361-6528/aa700e](https://doi.org/10.1088/1361-6528/aa700e).
- 142 P. W. May, M. Clegg, T. A. Silva, H. Zanin, O. Fatibello-Filho and V. Celorrio, *et al.*, Diamond-coated ‘black silicon’ as a promising material for high-surface-area electrochemical electrodes and antibacterial surfaces, *J. Mater. Chem. B*, 2016, **4**(34), 5737–5746, DOI: [10.1039/C6TB01774F](https://doi.org/10.1039/C6TB01774F).
- 143 L. E. Fisher, Y. Yang, M. F. Yuen, W. Zhang, A. H. Nobbs and B. Su, Bactericidal activity of biomimetic diamond nanocone surfaces, *Biointerphases*, 2016, **11**, 011014, DOI: [10.1116/1.4944062](https://doi.org/10.1116/1.4944062).
- 144 C. M. Bhadra, V. Khanh Truong, V. T. H. Pham, M. Al Kobaisi, G. Seniutinas and J. Y. Wang, *et al.*, Antibacterial titanium nano-patterned arrays inspired by dragonfly wings, *Sci. Rep.*, 2015, **5**(1), 16817, DOI: [10.1038/srep16817](https://doi.org/10.1038/srep16817).
- 145 C. Sengstock, M. Lopian, Y. Motemani, A. Borgmann, C. Khare and P. J. S. Buenconsejo, *et al.*, Structure-related antibacterial activity of a titanium nanostructured surface fabricated by glancing angle sputter deposition, *Nanotechnology*, 2014, **25**(19), 195101, DOI: [10.1088/0957-4484/25/19/195101](https://doi.org/10.1088/0957-4484/25/19/195101).
- 146 F. Hizal, I. Zhuk, S. Sukhishvili, H. J. Busscher, H. C. van der Mei and C. H. Choi, Impact of 3D Hierarchical Nanostructures on the Antibacterial Efficacy of a Bacteria-Triggered Self-Defensive Antibiotic Coating, *ACS Appl. Mater. Interfaces*, 2015, **7**(36), 20304–20313, DOI: [10.1021/acsami.5b05947](https://doi.org/10.1021/acsami.5b05947).
- 147 T. Sjöström, A. H. Nobbs and B. Su, Bactericidal nanospire surfaces via thermal oxidation of Ti alloy substrates, *Mater. Lett.*, 2016, **167**, 22–26, DOI: [10.1016/j.matlet.2015.12.140](https://doi.org/10.1016/j.matlet.2015.12.140).
- 148 T. Diu, N. Faruqui, T. Sjöström, B. Lamarre, H. F. Jenkinson and B. Su, *et al.*, Cicada-inspired cell-instructive

- nanopatterned arrays, *Sci. Rep.*, 2014, 4(1), 7122, DOI: [10.1038/srep07122](https://doi.org/10.1038/srep07122).
- 149 X. Ge, C. Ren, Y. Ding, G. Chen, X. Lu and K. Wang, *et al.*, Micro/nano-structured TiO₂ surface with dual-functional antibacterial effects for biomedical applications, *Bioact. Mater.*, 2019, 4, 346–357, DOI: [10.1016/j.bioactmat.2019.10.006](https://doi.org/10.1016/j.bioactmat.2019.10.006).
- 150 J. Hasan, Y. Xu, T. Yarlagadda, M. Schuetz, K. Spann and P. K. Yarlagadda, Antiviral and Antibacterial Nanostructured Surfaces with Excellent Mechanical Properties for Hospital Applications, *ACS Biomater. Sci. Eng.*, 2020, 6(6), 3608–3618, DOI: [10.1021/acsbiomaterials.0c00348](https://doi.org/10.1021/acsbiomaterials.0c00348).
- 151 M. N. Dickson, E. I. Liang, L. A. Rodriguez, N. Vollereaux and A. F. Yee, Nanopatterned polymer surfaces with bactericidal properties, *Biointerphases*, 2015, 10(2), 021010, DOI: [10.1116/1.4922157](https://doi.org/10.1116/1.4922157).
- 152 M. Nerantzaki, N. Kehagias, A. Francone, A. Fernández, C. M. Sotomayor Torres and R. Papi, *et al.*, Design of a Multifunctional Nanoengineered PLLA Surface by Maximizing the Synergies between Biochemical and Surface Design Bactericidal Effects, *ACS Omega*, 2018, 3(2), 1509–1521, DOI: [10.1021/acsomega.7b01756](https://doi.org/10.1021/acsomega.7b01756).
- 153 Q. Cui, T. Liu, X. Li, K. Song and D. Ge, Nanopillared Polycarbonate Surfaces Having Variable Feature Parameters as Bactericidal Coatings, *ACS Appl. Nano Mater.*, 2020, 3(5), 4599–4609, DOI: [10.1021/acsanm.0c00645](https://doi.org/10.1021/acsanm.0c00645).
- 154 D. W. Green, K. K. H. Lee, J. A. Watson, H. Y. Kim, K. S. Yoon and E. J. Kim, *et al.*, High Quality Bioreplication of Intricate Nanostructures from a Fragile Gecko Skin Surface with Bactericidal Properties, *Sci. Rep.*, 2017, 7(1), 41023, DOI: [10.1038/srep41023](https://doi.org/10.1038/srep41023).
- 155 S. Wu, F. Zuber, J. Brugger, K. Maniura-Weber and Q. Ren, Antibacterial Au nanostructured surfaces, *Nanoscale*, 2016, 8(5), 2620–2625, DOI: [10.1039/C5NR06157A](https://doi.org/10.1039/C5NR06157A).
- 156 M. T. Alameda, M. R. Osorio, J. J. Hernández and I. Rodríguez, Hierarchical micro-nano topographies to control Bacteria and mesenchymal stem cells biological responses, *Sci. Rep.*, 2025, 15(1), 25405, DOI: [10.1038/s41598-025-08415-2](https://doi.org/10.1038/s41598-025-08415-2).
- 157 M. Kargar, A. Pruden and W. A. Ducker, Preventing bacterial colonization using colloidal crystals, *J. Mater. Chem. B*, 2014, 2(36), 5962–5971, DOI: [10.1039/C4TB00835A](https://doi.org/10.1039/C4TB00835A).
- 158 G. Feng, Y. Cheng, S. Y. Wang, D. A. Borca-Tasciuc, R. W. Worobo and C. I. Moraru, Bacterial attachment and biofilm formation on surfaces are reduced by small-diameter nanoscale pores: how small is small enough?, *npj Biofilms Microbiomes*, 2015, 1(1), 15022, DOI: [10.1038/npjbiofilms.2015.22](https://doi.org/10.1038/npjbiofilms.2015.22).
- 159 P. C. Hsieh and H. W. Chien, Biomimetic surfaces: Insights on the role of surface topography and wetting properties in bacterial attachment and biofilm formation, *Colloids Surf., B*, 2023, 228, 113389, DOI: [10.1016/j.colsurfb.2023.113389](https://doi.org/10.1016/j.colsurfb.2023.113389).
- 160 R. Mok, J. Dunkel and V. Kantsler, Geometric control of bacterial surface accumulation, *Phys. Rev. E*, 2019, 99(5), 052607, DOI: [10.1103/PhysRevE.99.052607](https://doi.org/10.1103/PhysRevE.99.052607).
- 161 H. Gu, K. W. Kolewe and D. Ren, Conjugation in *Escherichia coli* Biofilms on Poly(dimethylsiloxane) Surfaces with Microtopographic Patterns, *Langmuir*, 2017, 33(12), 3142–3150, DOI: [10.1021/acs.langmuir.6b04679](https://doi.org/10.1021/acs.langmuir.6b04679).
- 162 H. Gu, A. Chen, X. Song, M. E. Brasch, J. H. Henderson and D. Ren, How *Escherichia coli* lands and forms cell clusters on a surface: a new role of surface topography, *Sci. Rep.*, 2016, 6(1), 29516, DOI: [10.1038/srep29516](https://doi.org/10.1038/srep29516).
- 163 D. P. Linklater, V. A. Baulin, S. Juodkakis, R. J. Crawford, P. Stoodley and E. P. Ivanova, Mechano-bactericidal actions of nanostructured surfaces, *Nat. Rev. Microbiol.*, 2021, 19(1), 8–22, DOI: [10.1038/s41579-020-0414-z](https://doi.org/10.1038/s41579-020-0414-z).
- 164 D. Wijethunge, A. Mathew and P. K. D. V. Yarlagadda, Comprehensive review of bacterial death mechanism on nanopillared nanostructured surfaces, *Biophys. Rev.*, 2025, 17(3), 893–908, DOI: [10.1007/s12551-025-01319-5](https://doi.org/10.1007/s12551-025-01319-5).
- 165 D. P. Linklater and E. P. Ivanova, Nanostructured antibacterial surfaces – What can be achieved?, *Nano Today*, 2022, 43, 101404, DOI: [10.1016/j.nantod.2022.101404](https://doi.org/10.1016/j.nantod.2022.101404).
- 166 A. Uneputti, A. Dávila-Lezama, D. Garibo, A. Oknianska, N. Bogdanchikova and J. F. Hernández-Sánchez, *et al.*, Strategies applied to modify structured and smooth surfaces: A step closer to reduce bacterial adhesion and biofilm formation, *Colloid Interface Sci. Commun.*, 2022, 46, 100560, DOI: [10.1016/j.colcom.2021.100560](https://doi.org/10.1016/j.colcom.2021.100560).
- 167 S. Wu, F. Zuber, K. Maniura-Weber, J. Brugger and Q. Ren, Nanostructured surface topographies have an effect on bactericidal activity, *J. Nanobiotechnol.*, 2018, 16(1), 20, DOI: [10.1186/s12951-018-0347-0](https://doi.org/10.1186/s12951-018-0347-0).
- 168 X. Zhang, L. Wang and E. Levänen, Superhydrophobic surfaces for the reduction of bacterial adhesion, *RSC Adv.*, 2013, 3(30), 12003, DOI: [10.1039/c3ra40497h](https://doi.org/10.1039/c3ra40497h).
- 169 J. Drelich, E. Chibowski, D. D. Meng and K. Terpilowski, Hydrophilic and superhydrophilic surfaces and materials, *Soft Matter*, 2011, 7(21), 9804, DOI: [10.1039/c1sm05849e](https://doi.org/10.1039/c1sm05849e).
- 170 F. Hizal, N. Rungraeng, J. Lee, S. Jun, H. J. Busscher and H. C. van der Mei, *et al.*, Nanoengineered Superhydrophobic Surfaces of Aluminum with Extremely Low Bacterial Adhesivity, *ACS Appl. Mater. Interfaces*, 2017, 9(13), 12118–12129, DOI: [10.1021/acsami.7b01322](https://doi.org/10.1021/acsami.7b01322).
- 171 K. Ellinas, D. Kefallinou, K. Stamatakis, E. Gogolides and A. Tserepi, Is There a Threshold in the Antibacterial Action of Superhydrophobic Surfaces?, *ACS Appl. Mater. Interfaces*, 2017, 9(45), 39781–39789, DOI: [10.1021/acsami.7b11402](https://doi.org/10.1021/acsami.7b11402).
- 172 S. T. Rutherford and B. L. Bassler, Bacterial Quorum Sensing: Its Role in Virulence and Possibilities for Its Control, *Cold Spring Harbor Perspect. Med.*, 2012, 2(11), a012427, DOI: [10.1101/cshperspect.a012427](https://doi.org/10.1101/cshperspect.a012427).
- 173 R. Cuahtecotzi Delint, M. I. Ishak, P. M. Tsimbouri, V. Jayawarna, K. V. E. Burgess and G. Ramage, *et al.*, Nanotopography Influences Host–Pathogen Quorum Sensing and Facilitates Selection of Bioactive Metabolites in Mesenchymal Stromal Cells and *Pseudomonas aeruginosa* Co-Cultures, *ACS Appl. Mater. Interfaces*, 2024, 16(33), 43374–43386, DOI: [10.1021/acsami.4c09291](https://doi.org/10.1021/acsami.4c09291).

- 174 M. Romero, J. Luckett, J. F. Dubern, G. P. Figueredo, E. Ison and A. M. Carabelli, *et al.*, Combinatorial discovery of microtopographical landscapes that resist biofilm formation through quorum sensing mediated autolubrication, *Nat. Commun.*, 2025, **16**(1), 5295, DOI: [10.1038/s41467-025-60567-x](https://doi.org/10.1038/s41467-025-60567-x).
- 175 S. Mukherjee and B. L. Bassler, Bacterial quorum sensing in complex and dynamically changing environments, *Nat. Rev. Microbiol.*, 2019, **17**(6), 371–382, DOI: [10.1038/s41579-019-0186-5](https://doi.org/10.1038/s41579-019-0186-5).
- 176 A. Mishra, A. Aggarwal and F. Khan, Medical Device-Associated Infections Caused by Biofilm-Forming Microbial Pathogens and Controlling Strategies, *Antibiotics*, 2024, **13**(7), 623, DOI: [10.3390/antibiotics13070623](https://doi.org/10.3390/antibiotics13070623).
- 177 G. S. Prabhukhot, C. D. Eggleton, M. Kim and J. Patel, Impact of surface topography and hydrodynamic flow conditions on single and multispecies biofilm formation by *Escherichia coli* O157:H7 and *Listeria monocytogenes* in presence of promotor bacteria, *LWT-Food Sci. Technol.*, 2024, **201**, 116240, DOI: [10.1016/j.lwt.2024.116240](https://doi.org/10.1016/j.lwt.2024.116240).
- 178 L. Xu and C. A. Siedlecki, Submicron topography design for controlling staphylococcal bacterial adhesion and biofilm formation, *J. Biomed. Mater. Res., Part A*, 2022, **110**(6), 1238–1250, DOI: [10.1002/jbm.a.37369](https://doi.org/10.1002/jbm.a.37369).
- 179 T. Zhou, X. Wan, D. Z. Huang, Z. Li, Z. Peng and A. Anandkumar, *et al.*, AI-aided geometric design of anti-infection catheters, *Sci. Adv.*, 2024, **10**, eadj1741, DOI: [10.1126/sciadv.adj1741](https://doi.org/10.1126/sciadv.adj1741).
- 180 X. Ge, Y. Leng, X. Lu, F. Ren, K. Wang and Y. Ding, *et al.*, Bacterial responses to periodic micropillar array, *J. Biomed. Mater. Res., Part A*, 2015, **103**(1), 384–396, DOI: [10.1002/jbm.a.35182](https://doi.org/10.1002/jbm.a.35182).
- 181 E. Fadeeva, V. K. Truong, M. Stiesch, B. N. Chichkov, R. J. Crawford and J. Wang, *et al.*, Bacterial Retention on Superhydrophobic Titanium Surfaces Fabricated by Femtosecond Laser Ablation, *Langmuir*, 2011, **27**(6), 3012–3019, DOI: [10.1021/la104607g](https://doi.org/10.1021/la104607g).
- 182 F. Variola, S. Francis-Zalzal, A. Leduc, J. Barbeau and A. Nanci, Oxidative nanopatterning of titanium generates mesoporous surfaces with antimicrobial properties, *Int. J. Nanomed.*, 2014, 2319, DOI: [10.2147/IJN.S61333](https://doi.org/10.2147/IJN.S61333).
- 183 S. Kim, U. T. Jung, S. K. Kim, J. H. Lee, H. S. Choi and C. S. Kim, *et al.*, Nanostructured Multifunctional Surface with Antireflective and Antimicrobial Characteristics, *ACS Appl. Mater. Interfaces*, 2015, **7**(1), 326–331, DOI: [10.1021/am506254r](https://doi.org/10.1021/am506254r).
- 184 V. Vadillo-Rodríguez, A. I. Guerra-García-Mora, D. Perera-Costa, M. L. González-Martín and M. C. Fernández-Calderón, Bacterial response to spatially organized microtopographic surface patterns with nanometer scale roughness, *Colloids Surf., B*, 2018, **169**, 340–347, DOI: [10.1016/j.colsurfb.2018.05.038](https://doi.org/10.1016/j.colsurfb.2018.05.038).
- 185 S. Rostami, F. Puza, M. Ucak, E. Ozgur, O. Gul and U. K. Ercan, *et al.*, Bifunctional sharkskin mimicked chitosan/graphene oxide membranes: Reduced biofilm formation and improved cytocompatibility, *Appl. Surf. Sci.*, 2021, **544**, 148828, DOI: [10.1016/j.apsusc.2020.148828](https://doi.org/10.1016/j.apsusc.2020.148828).
- 186 C. Serrano, L. García-Fernández, J. P. Fernández-Blázquez, M. Barbeck, S. Ghanaati and R. Unger, *et al.*, Nanostructured medical sutures with antibacterial properties, *Biomaterials*, 2015, **52**, 291–300, DOI: [10.1016/j.biomaterials.2015.02.039](https://doi.org/10.1016/j.biomaterials.2015.02.039).
- 187 J. Valle, S. Burgui, D. Langheinrich, C. Gil, C. Solano and A. Toledo-Arana, *et al.*, Evaluation of Surface Microtopography Engineered by Direct Laser Interference for Bacterial Anti-Biofouling, *Macromol. Biosci.*, 2015, **15**(8), 1060–1069, DOI: [10.1002/mabi.201500107](https://doi.org/10.1002/mabi.201500107).
- 188 R. Elashnikov, P. Ulbrich, B. Vokatá, V. S. Pavlíčková, V. Švorčík and O. Lyutakov, *et al.*, Physically Switchable Antimicrobial Surfaces and Coatings: General Concept and Recent Achievements, *Nanomaterials*, 2021, **11**(11), 3083, DOI: [10.3390/nano11113083](https://doi.org/10.3390/nano11113083).
- 189 A. Uneputti, A. Dávila-Lezama, D. Garibo, A. Oknianska, N. Bogdanchikova and J. F. Hernández-Sánchez, *et al.*, Strategies applied to modify structured and smooth surfaces: A step closer to reduce bacterial adhesion and biofilm formation, *Colloid Interface Sci. Commun.*, 2022, **46**, 100560, DOI: [10.1016/j.colcom.2021.100560](https://doi.org/10.1016/j.colcom.2021.100560).
- 190 M. Zhang, Z. Yu and E. C. M. Lo, A New pH-Responsive Nano Micelle for Enhancing the Effect of a Hydrophobic Bactericidal Agent on Mature *Streptococcus mutans* Biofilm, *Front. Microbiol.*, 2021, **12**, 761583, DOI: [10.3389/fmicb.2021.761583](https://doi.org/10.3389/fmicb.2021.761583).
- 191 H. Gu, S. W. Lee, J. Carnicelli, T. Zhang and D. Ren, Magnetically driven active topography for long-term biofilm control, *Nat. Commun.*, 2020, **11**(1), 2211, DOI: [10.1038/s41467-020-16055-5](https://doi.org/10.1038/s41467-020-16055-5).
- 192 M. J. Oh, A. Babeer, Y. Liu, Z. Ren, J. Wu and D. A. Issadore, *et al.*, Surface Topography-Adaptive Robotic Superstructures for Biofilm Removal and Pathogen Detection on Human Teeth, *ACS Nano*, 2022, **16**(8), 11998–12012, DOI: [10.1021/acsnano.2c01950](https://doi.org/10.1021/acsnano.2c01950).
- 193 H. Wang, Z. Zhang, Z. Wang, Y. Liang, Z. Cui and J. Zhao, *et al.*, Multistimuli-Responsive Microstructured Superamphiphobic Surfaces with Large-Range, Reversible Switchable Wettability for Oil, *ACS Appl. Mater. Interfaces*, 2019, **11**(31), 28478–28486, DOI: [10.1021/acsami.9b07941](https://doi.org/10.1021/acsami.9b07941).
- 194 R. Elashnikov, O. Lyutakov, P. Ulbrich and V. Švorčík, Light-activated polymethylmethacrylate nanofibers with antibacterial activity, *Mater. Sci. Eng., C*, 2016, **64**, 229–235, DOI: [10.1016/j.msec.2016.03.047](https://doi.org/10.1016/j.msec.2016.03.047).
- 195 C. Yang, L. Wu and G. Li, Magnetically Responsive Superhydrophobic Surface: In Situ Reversible Switching of Water Droplet Wettability and Adhesion for Droplet Manipulation, *ACS Appl. Mater. Interfaces*, 2018, **10**(23), 20150–20158, DOI: [10.1021/acsami.8b04190](https://doi.org/10.1021/acsami.8b04190).
- 196 L. Děkanovský, R. Elashnikov, M. Kubíková, B. Vokatá, V. Švorčík and O. Lyutakov, Dual-Action Flexible Antimicrobial Material: Switchable Self-Cleaning, Antifouling, and Smart Drug Release, *Adv. Funct. Mater.*, 2019, **29**(31), 1–10, DOI: [10.1002/adfm.201901880](https://doi.org/10.1002/adfm.201901880).
- 197 S. Rajaramon, H. David, A. Sajeevan, K. Shanmugam, H. Sriramulu and R. Dandela, *et al.*, Multi-functional approach

- in the design of smart surfaces to mitigate bacterial infections: a review, *Front. Cell. Infect. Microbiol.*, 2023, **13**, 1–15, DOI: [10.3389/fcimb.2023.1139026](https://doi.org/10.3389/fcimb.2023.1139026).
- 198 Q. Su, Y. Xue, C. Wang, Q. Zhou, Y. Zhao and J. Su, *et al.*, Strategies and applications of antibacterial surface-modified biomaterials, *Bioact. Mater.*, 2025, **53**, 114–140, DOI: [10.1016/j.bioactmat.2025.07.009](https://doi.org/10.1016/j.bioactmat.2025.07.009).
 - 199 D. Perera-Costa, J. M. Bruque, M. L. González-Martín, A. C. Gómez-García and V. Vadillo-Rodríguez, Studying the Influence of Surface Topography on Bacterial Adhesion using Spatially Organized Microtopographic Surface Patterns, *Langmuir*, 2014, **30**(16), 4633–4641, DOI: [10.1021/la5001057](https://doi.org/10.1021/la5001057).
 - 200 E. Jin, Z. Lv, Y. Zhu, H. Zhang and H. Li, Nature-Inspired Micro/Nano-Structured Antibacterial Surfaces, *Molecules*, 2024, **29**(9), 1906, DOI: [10.3390/molecules29091906](https://doi.org/10.3390/molecules29091906).
 - 201 A. Thakur, R. Ganesan and D. J. Ray, Nanomaterials against antimicrobial resistance and beyond: toward mitigating bacterial resuscitation, *Total Environment Microbiology*, 2026, **2**(1), 100052, DOI: [10.1016/j.temicr.2025.100052](https://doi.org/10.1016/j.temicr.2025.100052).
 - 202 A. Jaggesar, H. Shahali, A. Mathew and P. K. D. V. Yarlagadda, Bio-mimicking nano and micro-structured surface fabrication for antibacterial properties in medical implants, *J. Nanobiotechnol.*, 2017, **15**(1), 64, DOI: [10.1186/s12951-017-0306-1](https://doi.org/10.1186/s12951-017-0306-1).
 - 203 R. Kaur and S. Liu, Antibacterial surface design – Contact kill, *Prog. Surf. Sci.*, 2016, **91**(3), 136–153, DOI: [10.1016/j.progsurf.2016.09.001](https://doi.org/10.1016/j.progsurf.2016.09.001).
 - 204 A. Soni and G. Brightwell, Nature-Inspired Antimicrobial Surfaces and Their Potential Applications in Food Industries, *Foods*, 2022, **11**(6), 844, DOI: [10.3390/foods11060844](https://doi.org/10.3390/foods11060844).
 - 205 K. Karimi, A. Fardoost, N. Mhatre, J. Rajan, D. Boisvert and M. Javanmard, A Thorough Review of Emerging Technologies in Micro- and Nanochannel Fabrication: Limitations, Applications, and Comparison, *Micromachines*, 2024, **15**(10), 1274, DOI: [10.3390/mi15101274](https://doi.org/10.3390/mi15101274).
 - 206 O. Sen, P. Poddar, P. Sarkar, S. Das and S. Manna, Current advancements in microneedle technology for therapeutic and biomedical applications, *Sens. Int.*, 2025, **6**, 100325, DOI: [10.1016/j.sintl.2024.100325](https://doi.org/10.1016/j.sintl.2024.100325).
 - 207 Y. Sun, Y. Yang, W. Jiang, H. Bai, H. Liu and J. Wang, In Vivo Antibacterial Efficacy of Nanopatterns on Titanium Implant Surface: A Systematic Review of the Literature, *Antibiotics*, 2021, **10**(12), 1524, DOI: [10.3390/antibiotics10121524](https://doi.org/10.3390/antibiotics10121524).
 - 208 N. Lin, P. Berton, C. Moraes, R. D. Rogers and N. Tufenkji, Nanodarts, nanoblades, and nanospikes: Mechano-bactericidal nanostructures and where to find them, *Adv. Colloid Interface Sci.*, 2018, **252**, 55–68, DOI: [10.1016/j.cis.2017.12.007](https://doi.org/10.1016/j.cis.2017.12.007).
 - 209 A. G. Abdelhamid and A. E. Yousef, Combating Bacterial Biofilms: Current and Emerging Antibiofilm Strategies for Treating Persistent Infections, *Antibiotics*, 2023, **12**(6), 1005, DOI: [10.3390/antibiotics12061005](https://doi.org/10.3390/antibiotics12061005).
 - 210 Y. Wang, Y. Dong, Y. Quan, S. Wackerow, A. Abdolvand and S. A. Zolotovskaya, *et al.*, Hybrid Antibacterial Surfaces: Combining Laser-Induced Periodic Surface Structures with Polydopamine-Chitosan-Silver Nanoparticle Nanocomposite Coating, *Adv. Mater. Interfaces*, 2025, **12**(6), 1–12, DOI: [10.1002/admi.202400660](https://doi.org/10.1002/admi.202400660).
 - 211 P. Liu, Y. Wu, K. Tang, B. Mehrjou, J. Tao and G. Wang, *et al.*, Enhanced antibacterial activity of polyphenol-bound microtopography by synergistic chemical and micro/nanomechanical effects, *Composites, Part B*, 2024, **280**, 111498, DOI: [10.1016/j.compositesb.2024.111498](https://doi.org/10.1016/j.compositesb.2024.111498).
 - 212 H. Durand, A. Whiteley, P. Mailley and G. Nonglaton, Combining Topography and Chemistry to Produce Antibiofouling Surfaces: A Review, *ACS Appl. Bio Mater.*, 2022, **5**(10), 4718–4740, DOI: [10.1021/acsabm.2c00586](https://doi.org/10.1021/acsabm.2c00586).
 - 213 I. Georgakopoulos-Soares, E. L. Papazoglou, P. Karmiris-Obratański, N. E. Karkalos and A. P. Markopoulos, Surface antibacterial properties enhanced through engineered textures and surface roughness: A review, *Colloids Surf., B*, 2023, **231**, 113584, DOI: [10.1016/j.colsurfb.2023.113584](https://doi.org/10.1016/j.colsurfb.2023.113584).
 - 214 H. Koo, R. N. Allan, R. P. Howlin, P. Stoodley and L. Hall-Stoodley, Targeting microbial biofilms: current and prospective therapeutic strategies, *Nat. Rev. Microbiol.*, 2017, **15**(12), 740–755, DOI: [10.1038/nrmicro.2017.99](https://doi.org/10.1038/nrmicro.2017.99).